

MP1764A
Error Detector
Operation Manual

Sixteenth Edition

Read this manual before using the equipment.
Keep this manual with the equipment.

ANRITSU CORPORATION

Safety Symbols

To prevent the risk of personal injury or loss related to equipment malfunction, Anritsu Corporation uses the following safety symbols to indicate safety-related information. Insure that you clearly understand the meanings of the symbols BEFORE using the equipment.

Some or all of the following five symbols may not be used on all Anritsu equipment. In addition, there may be other labels attached to products which are not shown in the diagrams in this manual.

Symbols used in manual

DANGER  This indicates a very dangerous procedure that could result in serious injury or death if not performed properly.

WARNING  This indicates a hazardous procedure that could result in serious injury or death if not performed properly.

CAUTION  This indicates a hazardous procedure or danger that could result in light-to-severe injury, or loss related to equipment malfunction, if proper precautions are not taken.

Safety Symbols Used on Equipment and in Manual

The following safety symbols are used inside or on the equipment near operation locations to provide information about safety items and operation precautions. Insure that you clearly understand the meanings of the symbols and take the necessary precautions BEFORE using the equipment.



This indicates a prohibited operation. The prohibited operation is indicated symbolically in or near the barred circle.



This indicates an obligatory safety precaution. The obligatory operation is indicated symbolically in or near the circle.



This indicates warning or caution. The contents are indicated symbolically in or near the triangle.



This indicates a note. The contents are described in the box.



These indicate that the marked part should be recycled.

MP1764A
Error Detector
Operation Manual

10 November 1994 (First Edition)
30 August 2002 (Sixteenth Edition)

Copyright © 1994-2002, ANRITSU CORPORATION.

All rights reserved. No part of this manual may be reproduced without the prior written permission of the publisher.

The contents of this manual may be changed without prior notice.

Printed in Japan

For Safety

WARNING



1. ALWAYS refer to the operation manual when working near locations at which the alert mark shown on the left is attached. If the operation, etc., is performed without heeding the advice in the operation manual, there is a risk of personal injury. In addition, the equipment performance may be reduced. Moreover, this alert mark is sometimes used with other marks and descriptions indicating other dangers.



or



Repair

WARNING

Falling Over

2. When supplying power to this equipment, connect the accessory 3-pin power cord to a 3-pin grounded power outlet. If a grounded 3-pin outlet is not available, before supplying power to the equipment, use a conversion adapter and ground the green wire, or connect the frame ground on the rear panel of the equipment to ground. If power is supplied without grounding the equipment, there is a risk of receiving a severe or fatal electric shock.
3. This equipment cannot be repaired by the user. DO NOT attempt to open the cabinet or to disassemble internal parts. Only Anritsu-trained service personnel or staff from your sales representative with a knowledge of electrical fire and shock hazards should service this equipment. There are high-voltage parts in this equipment presenting a risk of severe injury or fatal electric shock to untrained personnel. In addition, there is a risk of damage to precision parts.
4. This equipment should be used in the correct position. If the cabinet is turned on its side, etc., it will be unstable and may be damaged if it falls over as a result of receiving a slight mechanical shock.

For Safety

CAUTION

Changing Fuse

CAUTION 

1. Before changing the fuses, ALWAYS remove the power cord from the power outlet and replace the blown fuses. ALWAYS use new fuses of the type and rating specified on the fuse marking on the rear panel of the cabinet.

___T indicates a time-lag fuse.

___A or F___ A indicate a normal fusing type fuse.

There is risk of receiving a fatal electric shock if the fuses are replaced with the power cord connected.

Cleaning

2. Keep the power supply and cooling fan free of dust.
 - Clean the power inlet regularly. If dust accumulates around the power pins, there is a risk of fire.
 - Keep the cooling fan clean so that the ventilation holes are not obstructed. If the ventilation is obstructed, the cabinet may over-heat and catch fire.
3. Use two or more people to lift and move this equipment, or use a trolley. There is a risk of back injury, if this equipment is lifted by one person.

 CAUTION/注意

>18kg

HEAVY WEIGHT/重量物

For Safety

CAUTION

Storage media

This instrument uses floppy disks for storing data and programs.

Incorrect use of the floppy disks or errors can cause the data stored on the medium to be erased. Back up the floppy disk as a precaution.

Anritsu will not compensate for loss of the stored data.

Note the following points when using this instrument. Especially, do not remove the floppy disk from the drive during disk access. For details, see the main text of this manual.

- Satisfy the specified environmental conditions. Do not use this instrument in places subject to dirt.
- Clean head of floppy disk drive with 3.5 inch head cleaning disk set regularly.
- Keep floppy disks away from magnetized products. Do not bend the floppy disk.

Disposing of the product

The MP1764A uses chemical compound semiconductor including arsenic and manganese dioxide Lithium Battery and timer including mercury. At the end of its life, the MP1764A should be recycled or disposed properly.

(Blank)

Equipment Certificate

Anritsu Corporation certifies that this equipment was tested before shipment using calibrated measuring instruments with direct traceability to public testing organizations recognized by national research laboratories including the Electrotechnical Laboratory, the National Research Laboratory of Metrology and the Communications Research Laboratory, and was found to meet the published specifications.

Anritsu Warranty

Anritsu Corporation will repair this equipment free-of-charge if a malfunction occurs within 1 year after shipment due to a manufacturing fault, provided that this warranty is rendered void under any or all of the following conditions.

- The fault is outside the scope of the warranty conditions described in the operation manual.
- The fault is due to mishandling, misuse, or unauthorized modification or repair of the equipment by the customer.
- The fault is due to severe usage clearly exceeding normal usage.
- The fault is due to improper or insufficient maintenance by the customer.
- The fault is due to natural disaster including fire, flooding, earthquake, etc.
- The fault is due to use of non-specified peripheral equipment, peripheral parts, consumables, etc.
- The fault is due to use of a non-specified power supply or in a non-specified installation location.

In addition, this warranty is valid only for the original equipment purchaser. It is not transferable if the equipment is resold.

Anritsu Corporation will not accept liability for equipment faults due to unforeseen and unusual circumstances, nor for faults due to mishandling by the customer.

Anritsu Corporation Contact

If this equipment develops a fault, contact Anritsu Corporation or its representatives at the address in this manual.

CE Marking

Anritsu affix the CE Conformity Marking on the following product(s) in accordance with the Council Directive 93/68/EEC to indicate that they conform with the EMC directive of the European Union (EU).

CE Conformity Marking



1. Product Name/Model Name

Product Name: Error Detector

Model Name: MP1764A

2. Applied Directive

EMC: Council Directive 89/336/EEC

Safety: Council Directive 73/23/EEC

3. Applied Standards

EMC :

Electromagnetic radiation:

EN55011(ISM, Group 1, Class A equipment)

Immunity:

EN50082-1

Performance Criteria*

IEC801-2 (ESD) 4 kVCD, 8 kVAD B

IEC801-3 (Rad.) 3 V/m A

IEC801-4 (EFT) 1 kV B

*: Performance Criteria

A: No performance degradation or function loss

B: Self-recovered temporary degradation of performance or temporary loss of function

Harmonic current emissions:

EN61000-3-2 (Class A equipment)

Safety: EN61010-1 (Installation Category II, Pollution Degree 2)

Power Line Fuse Protection


For safety, Anritsu products have either one or two fuses in the AC power lines as requested by the customer when ordering.

Single fuse: A fuse is inserted in one of the AC power lines.

Double fuse: A fuse is inserted in each of the AC power lines.


Example 1: An example of the single fuse is shown below:

Fuse Holder



Example 2: An example of the double fuse is shown below:

Fuse Holders

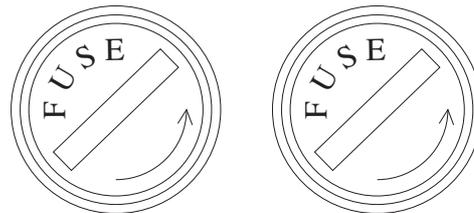

Title of Contents

For Safety	iii
SECTION 1 GENERAL	1-1
1.1 Features	1-1
1.2 Functions	1-2
1.3 Options	1-9
1.4 Composition	1-9
SECTION 2 PREPARATIONS	2-1
2.1 Installation Site Environment	2-1
2.2 Safety Measures	2-1
2.3 Power Supply Voltage	2-1
2.4 Internal Battery Life	2-1
2.5 Destruction Prevention Measures	2-2
SECTION 3 DESCRIPTION OF PANELS AND CONNECTORS	3-1
3.1 FRONT PANEL	3-2
3.2 REAR PANEL	3-4
SECTION 4 OPERATION	4-1
4.1 Setup	4-1
4.1.1 Measurement	4-2
4.2 Internal Memory Initialization	4-2
4.3 Input Conditions Setting	4-5
4.3.1 When both DATA and CLOCK are GND termination	4-6
4.3.2 When DATA and CLOCK are both ECL termination	4-8
4.3.3 Auto search	4-8
4.3.4 EYE MARGIN Measurement	4-9
4.4 Pattern Setting	4-10
4.4.1 Logic	4-12
4.4.2 Alternate pattern setting	4-12
4.4.3 Data pattern setting	4-14
4.4.4 Zero substitution pattern setting	4-15
4.4.5 Pseudo random pattern setting	4-16
4.4.6 Bit window setting	4-17
4.4.7 Block window setting	4-18

4.4.8	Sync detection mode	4-19
4.4.9	Tracking	4-21
4.4.10	Error analysis (Option 01)	4-22
4.5	Error Measurement	4-23
4.5.1	ERROR RATIO measurement	4-25
4.5.2	ERROR COUNT	4-26
4.5.3	ERROR INTERVAL	4-27
4.5.4	ERROR FREE INTERVAL	4-28
4.5.5	CLOCK FREQUENCY	4-29
4.5.6	DISPLAY display	4-30
4.5.7	Measurement mode selection	4-31
4.5.8	Measurement start/stop	4-31
4.5.9	Current data function	4-32
4.5.10	AUTO SYNC function	4-33
4.5.11	Measurement time setting	4-36
4.5.12	Real time setting	4-36
4.5.13	Error lamp and alarm lamps	4-37
4.5.14	Error detection mode setting	4-38
4.6	Memory (Floppy Disk)	4-39
4.6.1	File save	4-40
4.6.2	File recall	4-41
4.6.3	Disk formatting	4-41
4.6.4	File delete	4-42
4.6.5	Error messages	4-42
4.6.6	Floppy disk	4-43
4.6.7	Floppy disk precautions	4-43
4.7	Printer output	4-44
4.7.1	Printing Format	4-47
4.8	Definition of Terms	4-51
4.8.1	Measurement items	4-51
4.8.2	Alarm intervals	4-51
4.8.3	Threshold EI and EFI data	4-51
4.8.4	Error performance data	4-52
4.9	Processing of Measurement Data At Alarm Generation	4-54
4.10	FUNCTION Switch Setting	4-56

SECTION 5 PRINCIPLES OF OPERATION 5-1

5.1	Pseudorandom Pattern (PRBS Pattern)	5-1
5.2	Pattern Synchronized Output Synchronization	5-3
5.2.1	Pseudorandom pattern	5-3
5.2.2	Programmable pattern	5-3

	5.3	Frame Sync Output	5-4
	5.4	Error Output	5-5
SECTION 6		MEASUREMENT	6-1
	6.1	Set-up	6-1
	6.2	Measurement	6-1
	6.3	Burst Measurement	6-2
SECTION 7		PERFORMANCE CHECK	7-1
	7.1	When Performance Check Necessary	7-1
	7.2	Test Equipment	7-1
	7.3	Check Method	7-2
	7.3.1	Operating frequency	7-2
	7.3.2	Input data level	7-3
	7.3.3	Input clock level	7-4
	7.3.4	Pattern	7-5
	7.3.5	Measurement items	7-6
SECTION 8		MAINTENANCE	8-1
	8.1	Daily Maintenance	8-1
	8.2	Preparation for Shipment	8-1
SECTION 9		TROUBLESHOOTING AND REPAIR	9-1
	9.1	Before Considering Trouble	9-1
	9.2	Fuse Replacement	9-1

SECTION 1

GENERAL

1.1 Features

The MP1764A is an error detector that operates over the 50 MHz to 12.5 GHz frequency range, and is used in conjunction with an MP1763B Pulse Pattern Generator to test high-speed digital communication systems and high-speed semiconductors.



















The input threshold voltage (-3 V to $+1.875\text{ V}$) of MP1764A can be set in 1 mV steps and the input clock phase (-500 ps to $+500\text{ ps}$) can be set in 1 ps steps. The measurement patterns are pseudorandom (PRBS) pattern (1 period 2^N-1 ; $N=7, 9, 11, 15, 20, 21, 31$), programmable (PRGM) pattern (maximum 8M bits), alternate pattern, and zero substitution pattern. Since the 8M bits memory can program six STM-64 (OC192) frames, STM frame tests can be carried out by combining the MP1764A with an MP1763B Pulse Pattern Generator. The MP1764A has three error detection modes of total error, insertion error, and omission error. Its measurement items are error ratio, error count, error intervals (EI), error free intervals (EFI) and clock frequency. The measured result can be displayed on a display. A printer can printout the threshold EI/EFI data and performance data, as well as the measured result (error ratio, error count, EI/EFI, alarm time).

The MP1764A has an automatic search function that can automatically set the input data threshold voltage and input clock phase and a pattern tracking function that can send to and set the MP1764A pattern data to the MP1763B. The pattern tracking function can also send the MP1763B pattern data to the MP1764A. Data EYE Margin measurement is also possible. The MP1764A also has a memory function that can store the set patterns and pattern data to 3.5 inch floppy disk and read and set the stored data.

The MP1764A is equipped with an IEEE Std 488-1987 GPIB as standard so that it can be remotely controlled. It also has a DMA receive function that can receive pattern data transferred by DMA from the controller.

SECTION 1 GENERAL

1.2 Functions

Operating frequency		0.05 to 12.5 GHz												
Measurement pattern	PRBS	Pattern length	2^N-1 (N=7, 9, 11, 15, 20, 23, 31)											
		Mark ratio	1/2, 1/4, 1/8, 0/8 ($\overline{1/2}$, 3/4, 7/8, 8/8 possible by logic inversion)											
		Number of AND bit shifts at mark ratio	1 bit or 3 bits (switchable by rear panel DIP switch)											
	Zero substitution		Consecutive 0 pattern can be inserted up to pattern length-1. Pattern at zero substitution: 2^N (N=7, 9, 11, 15)											
	DATA	DATA length	2 to 8388608 bits 2 to 65536 bits : step 1 bit 65536 to 131072 bits : step 2 bits 131072 to 262144 bits : step 4 bits 262144 to 524288 bits : step 8 bits 524288 to 1048576 bits : step 16 bits 1048576 to 2097152 bits : step 32 bits 2097152 to 4194304 bits : step 64 bits 4194304 to 8388608 bits : step 128 bits											
		Editing function	All 0 / all 1 / page 0 / page 1											
	Alternate pattern	DATA length	128 to 4194304 bits / Step 128 bits (A/B same length)											
		Number of loops	Controlled by external signal											
		Editing function	All 0 / all 1 / page 0 / page 1											
	Logic inversion	Positive/Negative switching possible [PRBS] <table style="display: inline-table; vertical-align: middle; margin: 0 20px;"> <tr> <td style="text-align: center;">Positive</td> <td style="text-align: center;">Negative</td> </tr> <tr> <td>H </td> <td>H </td> </tr> <tr> <td>L </td> <td>L </td> </tr> </table> [PRGM] <table style="display: inline-table; vertical-align: middle; margin: 0 20px;"> <tr> <td style="text-align: center;">Positive</td> <td style="text-align: center;">Negative</td> </tr> <tr> <td>H </td> <td>H </td> </tr> <tr> <td>L </td> <td>L </td> </tr> </table>		Positive	Negative	H 	H 	L 	L 	Positive	Negative	H 	H 	L 
Positive	Negative													
H 	H 													
L 	L 													
Positive	Negative													
H 	H 													
L 	L 													

1.2 Functions

Synchronization method	Normal		Enabled when the measurement pattern is a zero substitution, DATA, or alternate pattern.
	Frame		Enabled when the measurement pattern is a zero substitution or alternate pattern, and when it is a DATA pattern and the data length is 128 bits or longer. Frame bit length: 4 to 32 bits in 4 bit steps Pattern A only for the alternate pattern.
	Quick		Enabled when the measurement pattern is a zero substitution, or DATA.
Measurement	Measurement items	Error detection mode	Insertion / omission / total
		Error ratio	0.0000×10^{-16} to 1.0000×10^{-0}
		Error count	0 to 9999999 and 1.0000×10^7 to 9.9999×10^{16}
		EI (asynchronous)	0 to 9999999 and 1.0000×10^7 to 9.9999×10^{16} Interval: 1 ms, 10 ms, 100 ms, 1 sec
		%EFI (asynchronous)	0.0000% to 100.0000%
		Frequency	0.05 to 12.5 GHz (resolution 1 kHz/accuracy 10 ppm+1 kHz)
	Measurement time	Gating	Single, repeat, untimed
		Gate time	1 sec to 99 days 23 hours 59 minutes 59 seconds
	Sync threshold value		Internal, 10^{-n} (n=2, 3, 4, 5, 6, 7, 8)
	Auto Sync	Automatic pattern synchronization function	YES
	Error performance calculation function		YES (ES, EFS, SES, DM, UAS) (Output to an external printer or GPIB)
	Current data		Cycle time: 0.1 sec, 0.2 sec Display : Interval / cycle (ER and EC only at cycle.)
	Auto search function		YES
	EYE margin measurement		YES
	Bit Window		1 to 32ch Each channel can be set independently.
	Error peripheral analysis function		YES (OPTION 01). However, this function is ineffective when the measurement pattern is an alternate pattern and when the QUICK synchronization method is used.
	External mask function		YES
Block window		YES (Effective only when the data length is a multiple of 32 and the QUICK synchronization method is not used.)	

SECTION 1 GENERAL

Input/output connector	Data input	Input waveform	NRZ
		Input amplitude	0.25 to 2.0 Vp-p
		Threshold voltage	-3.000 to 1.875 V (1mV steps)
		Termination voltage	GND / -2 V
		Input impedance	50 Ω
		Connector	APC-3.5
	Clock input	Input waveform	Up to 0.5 GHz: Square wave only (Duty 50%) Others : Sine wave or square wave (Duty 50%)
		Input amplitude	0.25 to 2.0 Vp-p
		Clock delay	± 500 ps (1ps step)
		Polarity switching	CLOCK / CLOCK
		Termination voltage	GND/-2 V
		Input impedance	50 Ω
		Connector	APC-3.5
	Sync signal output		1/32 Clock / Pattern sync (FIX) / Pattern sync (VARIABLE)
		Output level	V _{OH} : 0 ± 0.2 V Amplitude: 1 Vp-p ± 20%
		Connector	SMA
	Error output (DIRECT)	Output level	0 / -1 V ± 0.1 V (LOW level at error)
Connector		SMA	

1.2 Functions

Input/output connector	Error output (STRETCHED)	Output level	TTL (LOW level at error)
		Pulse width	350 ns ± 100 ns
		Connector	BNC
	Alarm output	Output condition	Clock loss, sync loss
		Output level	TTL (LOW level at alarm)
		Connector	BNC
	Frame sync output	Output level	0 / -1 V ± 0.1 V ^(*1)
		Connector	SMA
	Internal sync judgment output		HIGH level output when synchronization established.
		Output level	0 / -1 V ± 0.1 V
		Connector	SMA
	External mask input		Masked when LOW level.
		Input level	0 / -1 V ± 0.1 V
		Connector	SMA
	Resync input		Synchronization released when LOW level.
Input level		0 / -1 V ± 0.1 V	
Connector		SMA	
Pattern switching input		Alternate pattern A/B switching signal (A when LOW level)	
	Input level	ECL (H: -0.9 ± 0.2 V, L: -1.75 ± 0.2 V)	
	Connector	SMA	
Clock		Date and time display	

(*1) Frame sync output is output under the following conditions only:

- (1) When SYNC MODE is frame
- (2) When data length exceeds 128 bits

In short, it is not output for the PRBS pattern, when the data length is 128 bits, etc.

SECTION 1 GENERAL

Display	Measured result	7 segments, 8 digits display maximum
	Gating	12 segments bar graph
	Alarm	Error : Red LED Power failure history: Orange LED Clock loss: Orange LED Clock loss history : Orange LED Sync loss : Orange LED Sync loss history : Orange LED
Tracking function		YES
Audible alarm		YES (error sound, alarm sound)
Function switch		Functions conform to Table 1-1.
Parameter memory	Media	3.5 inch FDD 3 modes
	Format	See Table 1-2.
	Storage data	Programmable pattern / others
	Mode switching	Format, directory mode, recall, save, delete
Panel lock		Disables all keys other than POWER switch, LOCAL key, Printer and Alarm monitor.
External control		2 systems GPIB interface
	GPIB 1	Tracking and external controller connection port
	GPIB 2	External printer output port
Initialization		Initialization LOCAL key + POWER switch
Operating temperature range		0 to 50°C
Power requirement		AC100 V system: AC90 V to AC132 V AC200 V system: AC180 V to 250 V 47.5 to 63 Hz 800 VA maximum
Dimensions and weight		221.5±4H, 426±5W, 451±5D (mm), 35 kg maximum
Options	Option 01	Error analysis function

Table 1-1 Rear Panel FUNCTION DIP Switch Settings

① FUNCTION SW 1

S W	Function	Setting	
		0	1
1	Number of mark ratio AND bit shifts	1 bit	3 bit
2	Clock loss processing	OFF	ON
3	Sync loss processing	OFF	ON
4	Error performance threshold selection	10^{-3}	10^{-4}
5	Burst measurement	OFF	ON
6	Intermediate data calculation	OFF	ON
7 8	Error detection mode selection	* 1	* 1
9 10	Measurement interval time selection	* 2	* 2

* 1) SW7 SW8

0 0 : Total error
 0 1 : Insertion error
 1 0 : Omission error
 1 1 : Total error

* 2) SW9 SW10

0 0 : 1 msec
 0 1 : 10 msec
 1 0 : 100 msec
 1 1 : 1 sec

② FUNCTION SW 2

S W	Function	Setting	
		0	1
1	Data printing format	Standard	Abbreviated
2	Threshold EI, EFI data printing function selection	OFF	ON
3	Error performance data printing selection	OFF	ON
4	Intermediate data printing selection	OFF	ON
5	1 second data printing selection	OFF	ON
6 7	1 second data printing threshold selection	* 3	* 3
8	Paper saving	OFF	ON
9	Current data interval	100 ms	200 ms
10	FD format switching	* 4	* 4

* 3) SW6 SW7

0 0 : 0
 0 1 : 10^{-6}
 1 0 : 10^{-4}
 1 1 : 10^{-3}

* 4) Refer to table 1-2.

SECTION 1 GENERAL

Table 1-2

① 2HD

Type	Sector length [bytes/sector]	Number of sectors [sectors/track]	Number of tracks [tracks/side]	Number of sides	SW2 BIT 10
1232KB	1024	8	77	2	1
1440KB	512	18	80	2	0

② 2DD

Type	Sector length [bytes/sector]	Number of sectors [sectors/track]	Number of tracks [tracks/side]	Number of sides	SW2 BIT 10
640KB	512	8	80	2	1
720KB	512	9	80	2	0

1.3 Option

The following option is available with the MP1764A Error Detector.

OPTION 01 Error analysis function

1.4 Composition

The standard composition of the MP1764A Error Detector is shown in Table 1-3.

Table 1-3 MP1764A Standard Composition

Item	No.	Name	Qty	
Main Unit	MP1764A	MP1764A Error Detector	1	
Accessory	J0500A	Semirigid cable (50 cm)	2	APC • 3.5J-APC • 3.5J 13A (2.6 m) 408JE-102 MF51NR10A Formatted *1
	J0496	Conversion connector	2	
	J0515J	SMA cable (1 m)	3	
	J0491	Power cord w/shield	1	
	J0008	GPIB cable (2 m)	2	
	F0079	Fuse	2	
	Z0168	3.5 inch floppy disk (2HD)	2	
	M-W0887AE	Operation manual	1	
Z0481	12.5G/3.2G BERTS APPLICATION SOFTWARE DEMO	1		
Application parts	MB24B	Dolly		20A power cord/plug 2 pcs/set
	B0163	Transport quilting		
	B0171	Protective carrying case		
	B0044	Rack mounting kit 1MW.5U use		
	Z0416	3.5 inch head cleaning disk		

*1: The two 3.5 inch floppy disks are already formatted (1,440 kB). Patterns equivalent to PRBS²¹⁰-1 (mark ratios 1/2, 1/4, and 1/8) that can be generated by the MP1601A or MP1604A Pulse Pattern Generator from Anritsu Corporation are stored on one of these disks.

SECTION 1 GENERAL

(Blank)

SECTION 2 PREPARATIONS

2.1 Installation Site Environment

Do not use the instrument in locations:

- Where vibrations are severe.
- Where it is damp or dusty.
- Where there is exposure to direct sunlight.
- Where there is exposure to active gases.

Long-term storage at high temperatures will shorten the life of the internal battery. Store the instrument at normal room temperature.

Operating temperature and humidity conditions	0 to 50°C (However, 5°C to 40°C for floppy disks), Relative humidity ≤95%.
Storage temperature and humidity conditions	– 40 to 70°C, Relative humidity ≤95%.

2.2 Safety Measures

- Use the power cord to connect the ac power supply. Ground the ground terminal of the power cord or the frame ground terminal on the rear panel of the instrument.
- When changing the fuse, always use a fuse of the same rating. (See the fuse replacement section.)
- If the instrument is operated at room temperature after being used or stored for a long time at low temperature, condensation may occur and cause short-circuiting. To prevent this, do not turn the power on until the instrument is completely dry.

2.3 Power Supply Voltage

The power supply voltage for this instrument is shown on the rear panel. Use a voltage within the rated voltage range. Excessive voltage may damage the circuits.

2.4 Internal Battery Life

The MP1764A uses a lithium primary battery as the timer and memory back-up power supply. The life of this battery is 7 years or more when the instrument is stored at normal room temperature. However, since the battery life largely depends on the storage temperature, storage at high temperatures for long periods will shorten the period given above.


Since battery replacement can only be made by Anritsu, contact the nearest Anritsu representative when replacement is required.

SECTION 2 PREPARATIONS


2.5 Destruction Prevention Measures

- Do not apply excessive voltage to the input of this instrument. The circuits may be destroyed.
- Terminate the output into 50Ω . Do not feed current to the output. The load must be a 50Ω pure resistance termination at ground potential.
- Before connecting the input and output terminals, ground the other equipment (including test circuits) with a ground wire. (Static electric countermeasure)
- The outer and inner conductors of coaxial cable may be charged as a capacitor. Therefore, discharge them with a piece of metal, etc. before using the cable.
- This instrument contains hybrid ICs and other important circuits and parts. These parts are extremely vulnerable to static electricity. Never remove the bottom cover.
- The hybrid ICs inside this instrument are hermetically sealed. Never break this seal. If the hybrid ICs are unsealed and the instrument fails to perform as specified, maintenance may be refused.
- Ventilation holes are drilled into the bottom cover. Be careful not to block the ventilation.
- This instrument backs up, in internal memory, the setup conditions immediately before the power is turned on, but several seconds are necessary after setup is changed.

Note that if the power is turned off while internal memory is being updated, the setup state will be cleared (initialized).

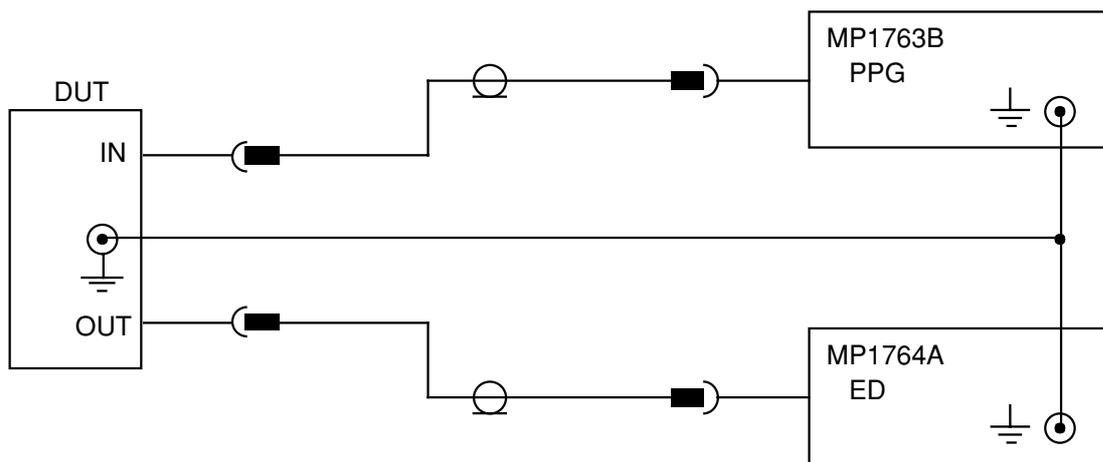

SECTION 3
DESCRIPTION OF PANELS AND CONNECTORS

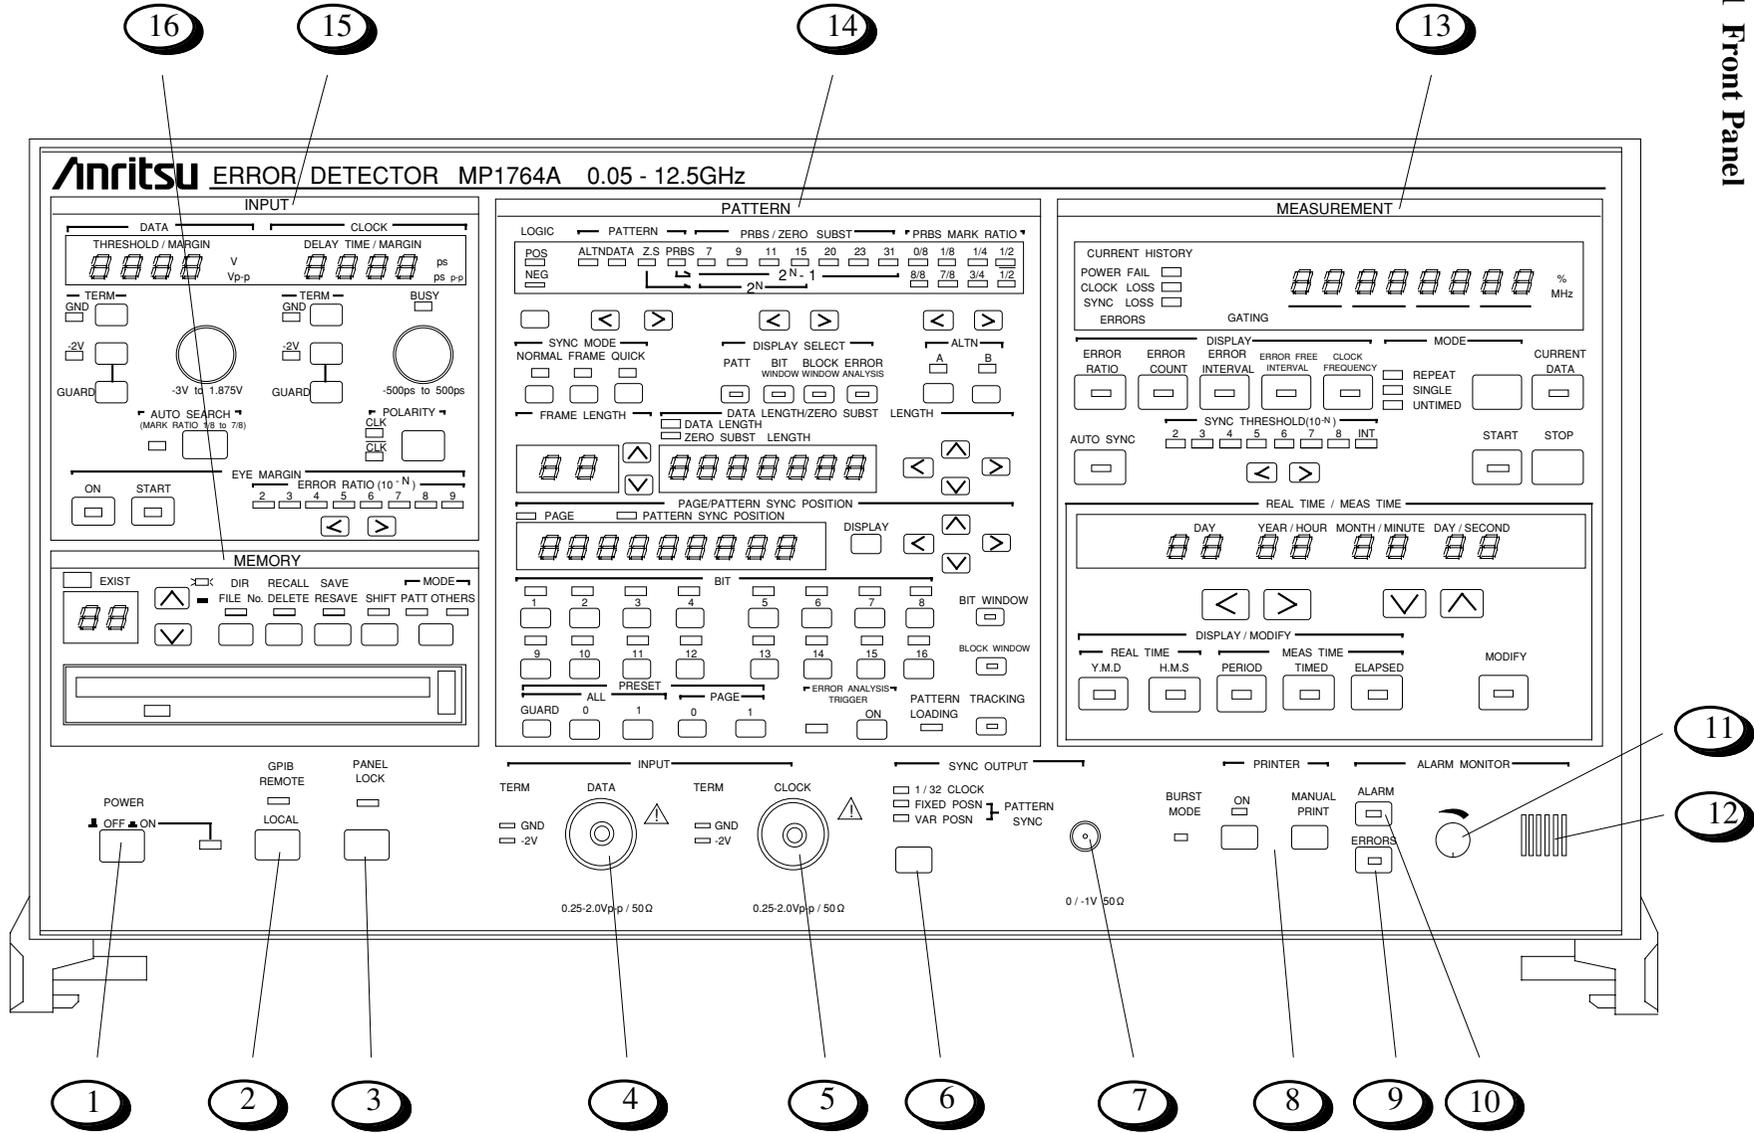

3.1 Front Panel


SECTION 3 DESCRIPTION OF PANELS AND CONNECTORS

11
12

1 2 3 4 5 6 7 8 9 10

SECTION 3 DESCRIPTION OF PANELS AND CONNECTORS

3.2 Rear Panel

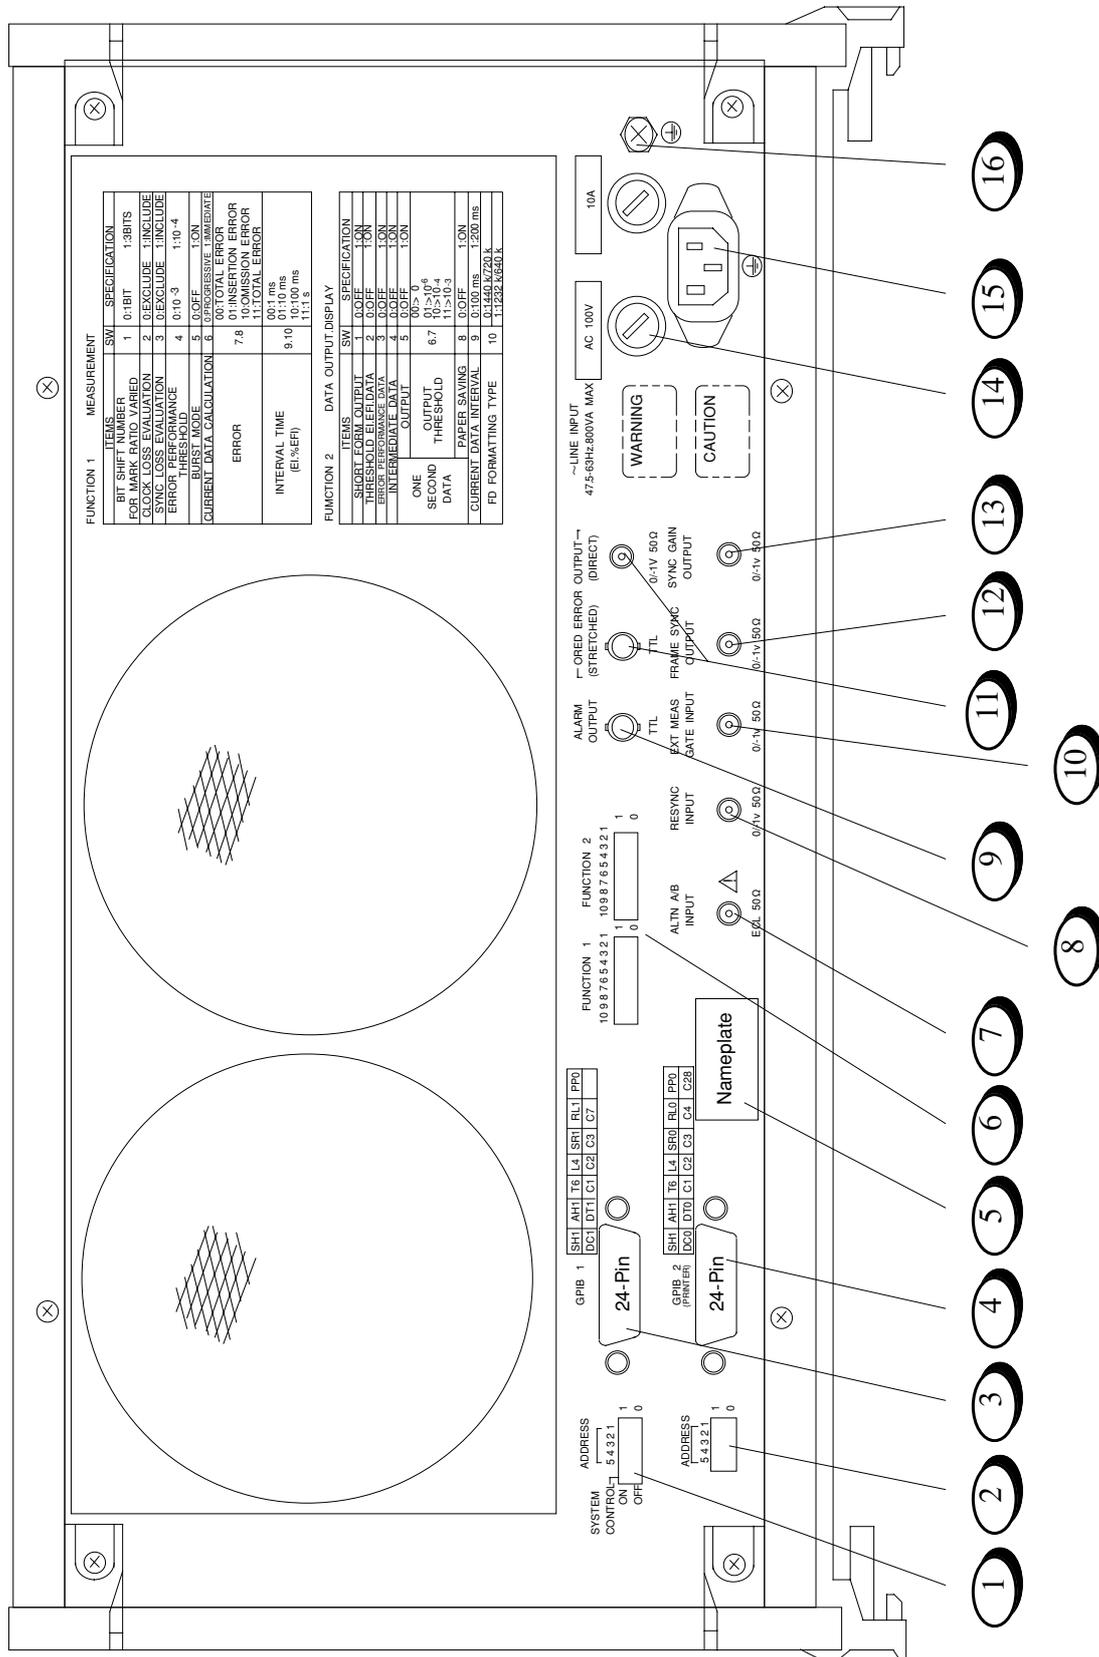

①	DIP switch	Sets system control ON/OFF and the GPIB 1 address.
②	DIP SWITCH	Sets the GPIB 2 address.
③	GPIB 1	GPIB 1 connector.
④	GPIB 2	GPIB 2 connector. (for printer)
⑤	Nameplate	Displays the serial number and option.
⑥	DIP SWITCH	FUNCTION 1/FUNCTION 2 setting DIP SWITCH.
⑦	ALT A/B INPUT	ECL level. Inputs the pattern A/pattern B switching timing in the ALTN mode.
⑧	RESYNC INPUT	0/-1 V 50Ω. When LOW level is input, sync loss is generated.
⑨	ALARM OUTPUT	TTL level. Outputs LOW level when an alarm is generated.
⑩	EXT MEAS GATE INPUT	0/-1 V 50Ω. Mask when LOW level.
⑪	ORED ERROR OUTPUT	STRETCHED: TTL level. Outputs low level when an error is generated. DIRECT: 0/-1 V 50Ω
⑫	FRAME SYNC OUTPUT	0/-1 V 50Ω
⑬	SYNC. GAIN OUTPUT	0/-1 V 50Ω. Synchronization established when HIGH level.
⑭	FUSE holder	
⑮	Power inlet	
⑯	Ground terminal	Connects to the ground terminal of the instrument connected to this instrument.


SECTION 3 DESCRIPTION OF PANELS AND CONNECTORS

(Blank)

SECTION 4 OPERATION

4.1 Setup


Be careful of static electricity when handling the MP1764A. Connection to an MP1763B Pulse Pattern Generator is described here as an example. Refer to the following figure and make the connections in the following order.

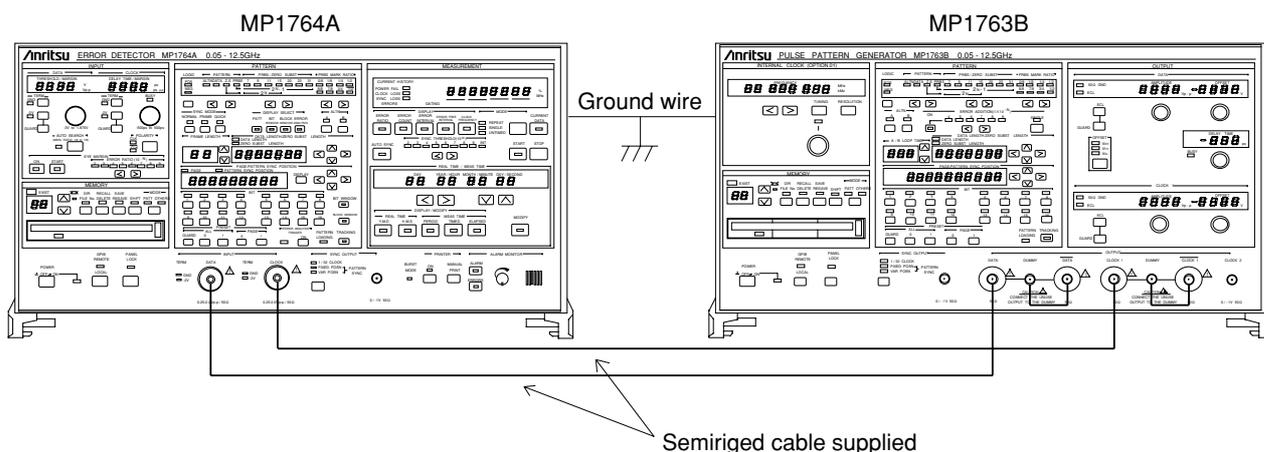

1. Connect the MP1764A and MP1763B ground terminals with ground wire.
2. Connect the power cord to an ac outlet. At this time, use a 3-prong plug with ground. If a 2-prong plug must be used, connect the MP1764A and MP1763B ground terminals before connecting the plug to the socket.
3. While pressing the LOCAL key, turn on the power and initialize the MP1764A and MP1763B. When initialization is performed, all the settings are set to the factory settings. (See Table 4-1.) When setting a pattern, etc. that you do not want to clear, save it to FD. (See 4.6.1.) Initialization makes the MP1764A and MP1763B settings the same. Turn off the power.

NOTE

If a high voltage is applied to the input connector, the protection circuit may be damaged. Never apply an input exceeding the rating. If the rating may be exceeded, check the input signal before making any connections.

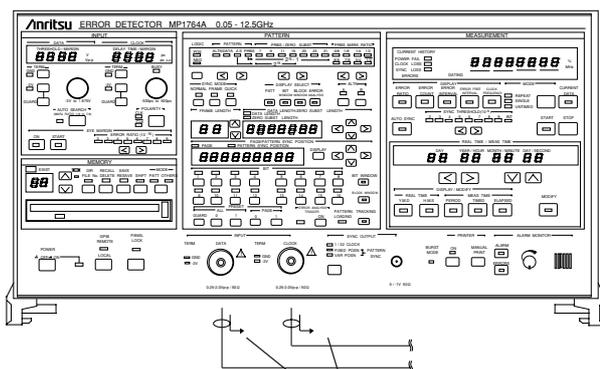

Don't forget level check!

Be careful of excessive input !


SECTION 4 OPERATION

4.1.1 Measurement

1. Check that the MP1764A Error Detector and MP1763B Pulse Pattern Generator settings are the same. Since the instruments were initialized in Paragraph 4.1, the settings should be the same. If the settings are different, initialize the instruments again. Then, set the MP1763B OUTPUT and the MP1764A AUTO SYNC to ON.
2. Press the MP1764A AUTO SEARCH key. The input data threshold voltage and input clock delay time are automatically set.

After the AUTO SEARCH lamp goes off, check that the CLOCK LOSS, SYNC LOSS, and ERRORS real time lamps are not lit. If the lamps are lit, check that signaling cables are connected correctly.

AUTO SEARCH key

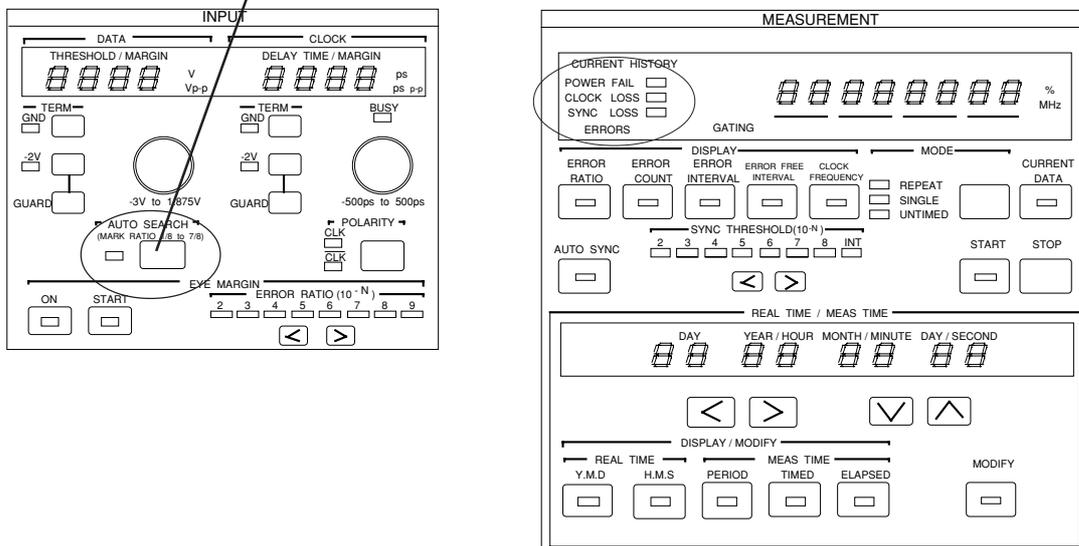

3. Change the DISPLAY display item and check if the following measured result is obtained:

ERROR RATIO : Error ratio displayed
 ERROR COUNT : Error count displayed
 ERROR INTERVAL : Number of error intervals (See 4.8.1.)
 ERROR FREE INTERVAL: Number of error free intervals ratio (See 4.8.1.)

4. Add an error and check if it is correctly detected.

Set MP1763B ERROR ADDITION to ON and select 1×10^{-6} .

Select ERROR RATIO at MP1764A DISPLAY and check if 1×10^{-6} is displayed at DISPLAY.

4.2 Internal Memory Initialization

To set the MP1764A to the initial state (factory setting state), set the POWER switch to ON while pressing the LOCAL key. When the MP1764A is set to the initial state, the previously set contents are all cleared and are preset as shown in Table 4-1. Verify which patterns, etc. must not be cleared with the user.

Table 4-1 Panel and Internal Circuits Initial State


Item		Panel	Internal circuit	
INPUT	DATA	TERM	GND	
		THRESHOLD value	-0.500	
	CLOCK	TERM	GND	
		DELAY TIME value	0	
		BUSY	OFF	
		POLARITY	CLK	
	AUTO SEARCH		OFF	
PATTERN	LOGIC		POS	
	PATTERN mode		PRBS 2 ¹⁵ -1	
	MARK RATIO		1/2	
	TRACKING		OFF	
	SYNC MODE		NORMAL	
	ALTN	Pattern		All 0
		A/B selection		A
		DATA LENGTH		128
		PAGE		1
	DATA	Pattern		All 0
		DATA LENGTH		2
		PAGE		1
	Z.S.	Pattern		Pseudo PRBS 2 ⁷
		ZERO SUB LENGTH		1
		PAGE		1
MEASURE- MENT	DISPLAY		ERROR RATIO (All digits "-" displayed on display)	
	CURRENT DATA		OFF	
	MODE		REPEAT	
	START		OFF	
	AUTO		OFF	
SYNC OUTPUT		1/32 CLOCK		
REAL TIME / MEAS TIME	Display		Measurement period is displayed. (1) REAL TIME • Y. M. D : Current date (year, month, day) • H. M. S : Current time (hour, minute, second) (2) MEAS TIME • PERIOD : 00 day 00 hour 00 minute 00 second • TIMED : All digits '-' • ELAPSED : All digits '-'	
	DISPLAY/MODIFY		PERIOD (MEAS TIME)	
	MODIFY		OFF	

SECTION 4 OPERATION

Table 4-1 Panel and Internal Circuits Initial State

Item		Panel	Internal circuits
GPIB REMOTE		OFF	
PANEL LOCK		OFF	
MEASURE CH MASK		Displayed according to the state at that time.	
PRINTER ON		OFF	
ALARM MONITOR	ALARM	OFF	
	ERRORS	OFF	
GPIB 1	ADDRESS 1 to 5	In accordance with the initial state of the switches.	
	SYSTEM CONTROL		
GPIB 2	ADDRESS 1 to 5		
FUNCTION 1			
FUNCTION 2			


4.3 Input Conditions Setting

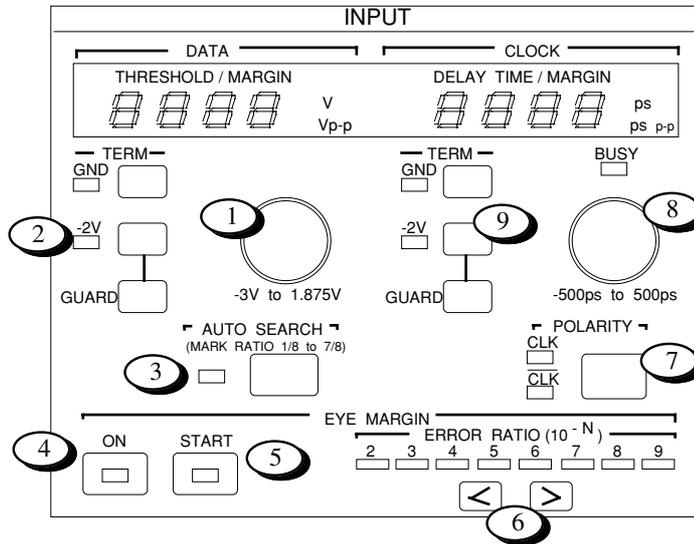

- | | | |
|---|------------------------|--|
| ① | Rotary encoder (DATA) | Sets the DATA THRESHOLD. |
| ② | TERM key | Selects the DATA termination condition. To select -2 V termination, press this key while pressing the GUARD key. |
| ③ | AUTO SEARCH key | Performs AUTO SEARCH. To repeat AUTO SEARCH, press this key again. |
| ④ | EYE MARGIN ON | Sets the EYE margin measurement mode. |
| ⑤ | EYE MARGIN START | Starts EYE margin measurement. |
| ⑥ | EYE MARGIN keys | Select the EYE margin threshold value. |
| ⑦ | POLARITY | Inverts the CLOCK polarity. |
| ⑧ | Rotary encoder (CLOCK) | Adjusts the CLOCK input phase within a ± 500 ps range. |
| ⑨ | TERM key | Selects the CLOCK termination conditions. To select -2 V termination, press this key while pressing the GUARD key. |

SECTION 4 OPERATION

4.3.1 When both DATA and CLOCK are GND termination

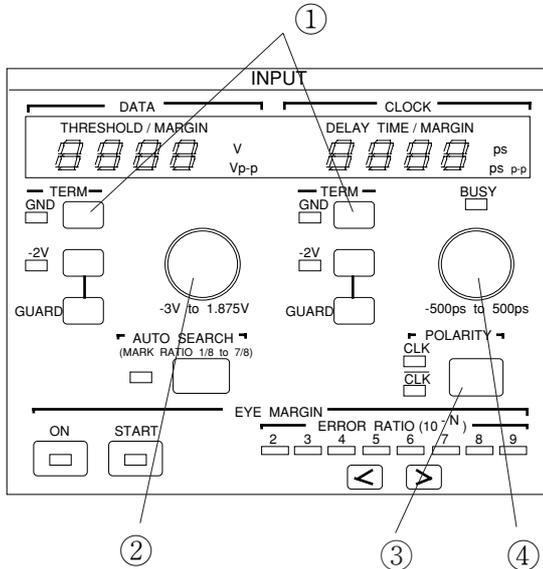

- ① Press the GND key. The GND LED lights.
- ② Turn the DATA rotary encoder and set the DATA threshold value. (See Fig. 4-1-1 to 4-1-3.)
- ③ Change the CLOCK polarity according to the DATA and clock input phase. (By synchronization relationship. See Fig. 4-2.)
- ④ Adjust the clock delay time.
Turn the rotary encoder and search for the error-free point. Set the delay time to midway between the two points that generate an error.

Example: When an error was generated at -210 ps and -130 ps, set the delay time to -170 ps.

- When amplitude and offset voltage known

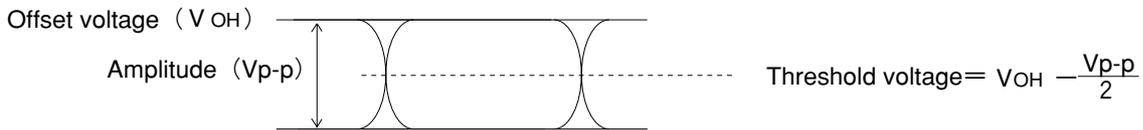


Fig. 4-1-1

- When high level and low level known

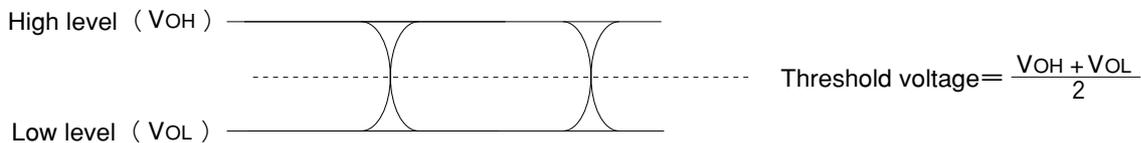


Fig. 4-1-2

4.3 Input Conditions Setting

Setting the optimum value

In the error free state, lower the DATA threshold voltage and measure the voltage that generates an error (V_1). Then raise the threshold voltage and measure the voltage that generates an error (V_2). Set the threshold voltage to midway between these two voltages. $\left(\frac{V_1 + V_2}{2}\right)$

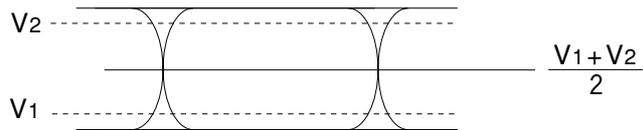


Fig. 4-1-3

Next, move CLOCK Delay in the minus direction and measure the phase (D_1) that generates an error. Then move CLOCK Delay in the plus direction and measure the phase (D_2) that generates an error. Set the CLOCK Delay to midway between these two values. $\left(\frac{D_1 + D_2}{2}\right)$


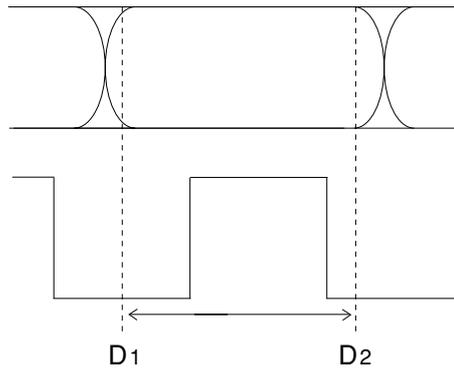


Fig. 4-2

SECTION 4 OPERATION

4.3.2 When DATA and CLOCK are both ECL termination

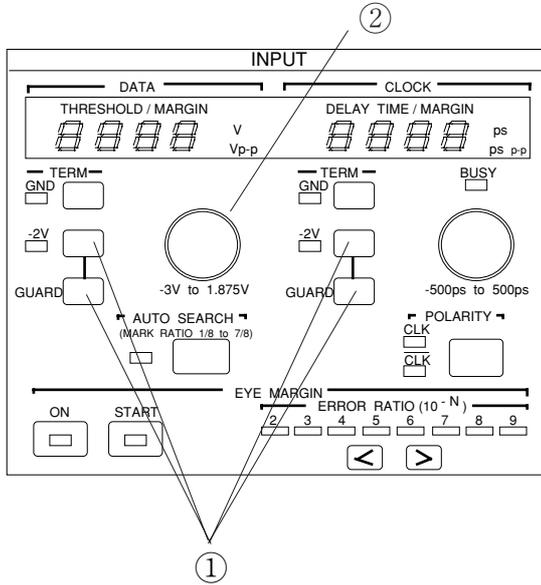


- ① While pressing the GUARD key, press the -2 V key. The -2 V LED lights.
- ② Set the DATA threshold voltage to -1.3 V (ECL standard voltage).
- ③ Set the CLOCK phase, etc. as described in Paragraph 4.3.1.

NOTE

Incorrect setting of the termination voltage may damage the device under test. Be very careful when changing the setting.


4.3.3 Auto search

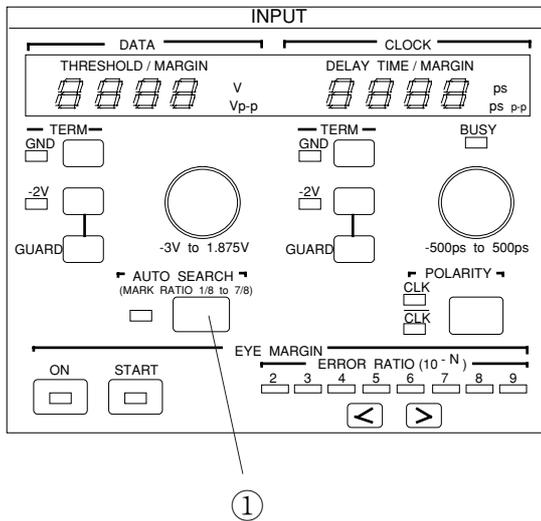


- ① When the AUTO SEARCH key is pressed, the DATA threshold voltage and CLOCK Delay are automatically set. If AUTO SEARCH does not end within three seconds, AUTO SEARCH stops and the AUTO SEARCH lamp begins to blink. At this time, return the data threshold voltage and CLOCK delay time to the set value before AUTO SEARCH.

If AUTO SEARCH does not end normally, check the cable connections and termination conditions. If they are normal, check the input waveform with a sampling oscilloscope.

4.3.4 EYE MARGIN Measurement

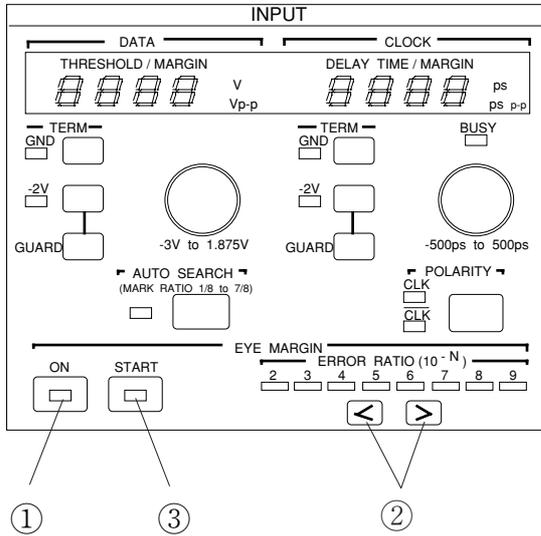


- ① Press the ON key. The LED inside the key lights. At this time,



is displayed.

- ② Set the threshold value error rate.
- ③ Start measurement by pressing the START key. At the end of measurement, the measured result is displayed on the display.


EYE MARGIN starts measurement from the point (point A) obtained by AUTO SEARCH. Therefore, measurements are made within the range shown below.

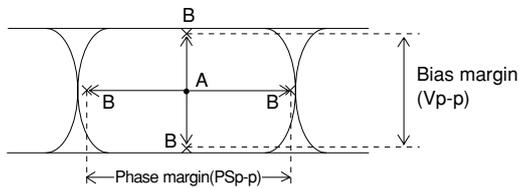



Point B is the position (10^{-2} to 10^{-9}) delayed by the threshold value set ERROR RATIO.

SECTION 4 OPERATION

4.4 Pattern Setting

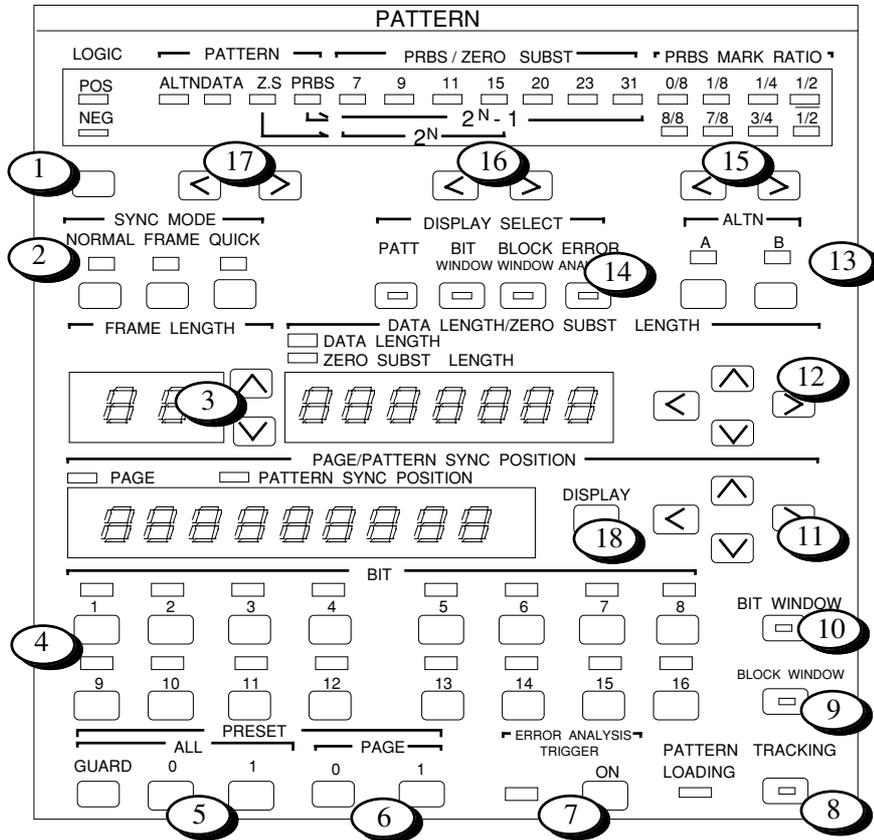


4.4 Pattern Setting

- | | |
|---|---|
| <p>① LOGIC</p> | <p>Inverts the DATA/DATA output logic. The DATA output logic is shown by lighting of the POS or NEG lamp.</p> |
| <p>② SYNC MODE</p> | <p>Selects the sync pull-in mode. One of the following three modes can be selected:</p> <p style="margin-left: 40px;">NORMAL : Turn on normal sync pull-in.
 FRAME : Turn on the frame sync function.
 QUICK : Turn on the quick sync function.</p> |
| <p>③ FRAME LENGTH</p> | <p>Sets the frame pattern bit length at FRAME SYNC .</p> |
| <p>④ BIT setting keys</p> | <p>Set the logic of each bit for each Page. When LOGIC is POS, lighting of the lamp above each key indicates logic '1'.</p> |
| <p>⑤ ALL edit keys</p> | <p>Set all the bits of the selected pattern to logic '0' or '1'. Press the 0 or 1 key while pressing the GUARD key.</p> |
| <p>⑥ PAGE edit keys</p> | <p>Set all bits of the displayed page to logic '0' or '1'.</p> |
| <p>⑦ ERROR ANALYSIS (OPTION 01)</p> | <p>Turns the error analysis function on and off. Lighting of the lamp shows that the error analysis function is 'ON'. This function is enabled only when OPTION 01 is built-in.</p> |
| <p>⑧ TRACKING</p> | <p>Turns the tracking function on and off. Lighting of the lamp inside the key shows that the tracking function is 'ON'.</p> |
| <p>⑨ BLOCK WINDOW</p> | <p>Turned on when error measurement in block units (32 bits) is masked.</p> |
| <p>⑩ BIT WINDOW</p> | <p>Turned on when error measurement in channel units (1 bit) is masked. (All 32 channels)</p> |
| <p>⑪  keys</p> | <p>Set the page and the pattern sync output position.</p> |
| <p>⑫  keys</p> | <p>Set the data length and number of consecutive zeros in Z.S.</p> |
| <p>⑬ ALTN keys</p> | <p>Select the A/B pattern at ALTN pattern setting.</p> |
| <p>⑭ DISPLAY SELECT</p> | <p>Select the item displayed on the display. When PATT, BIT WINDOW, and BLOCK WINDOW are set, that item is selected and is set at the panel. (It is possible to select ERROR ANALYSIS, When OPTION 01 is built-in.)</p> |
| <p>⑮ MARK ratio selection keys</p> | <p>Set the receive pattern mark ratio for PRBS.</p> |
| <p>⑯ PRBS/ZERO SUBST keys</p> | <p>Set the PRBS or pseudo PRBS period.</p> |
| <p>⑰ PATTERN selection keys</p> | <p>Select the type of receive pattern.</p> |
| <p>⑱ DISPLAY key</p> | <p>Toggles the display between PAGE and PATTERN SYNC POSITION. Selected display mode is displayed by the indicator.</p> |


SECTION 4 OPERATION

4.4.1 Logic

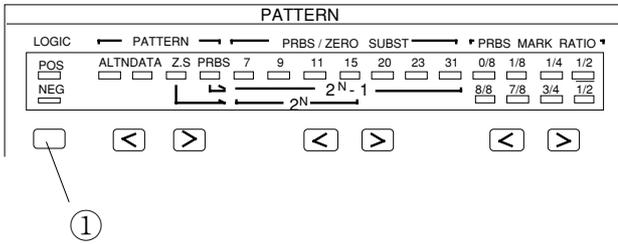

- ① Each time the LOGIC key is pressed, the logic of the set pattern changes in positive → negative → positive order. (The set logic is shown by lighting of the lamps.)

4.4.2 Alternate pattern setting

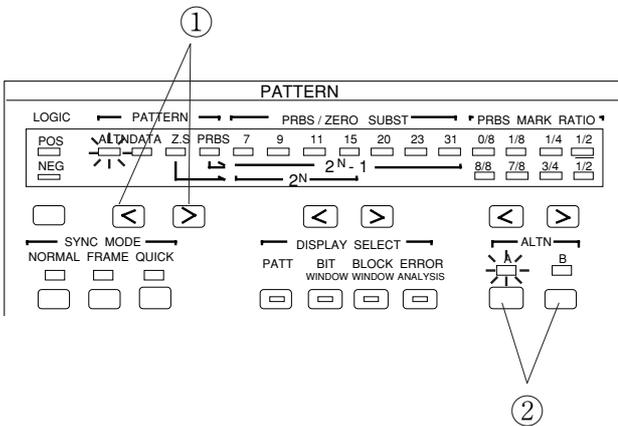


- ① Select ALTN with the keys.

DATA, Z.S., and PRBS are selected with these keys.

ALTN → DATA → Z.S. → PRBS

ALTN ← DATA ← Z.S. ← PRBS

- ② Pattern A or B is selected with this key. First, pattern A is set and A lights. (Either pattern A or pattern B can be set first.)

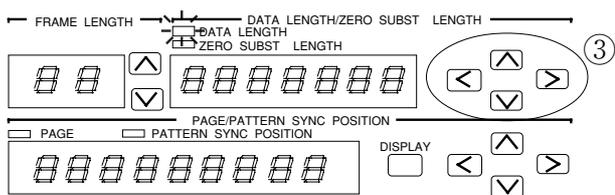


- ③ Set DATA LENGTH with the and keys. This value is common to both patterns A and B.

Select the digit to be set with the keys.

Set DATA LENGTH with the keys.

Set value: 128 to 4194304 bits (128 bit steps)

4.4 Pattern Setting

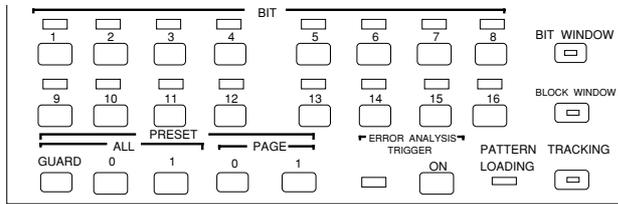

Change the BIT value with the button below the LED. When LOGIC is positive, lighting of the LED indicates High Level.

When you want to change all the DATA at once, use PRESET ALL or PAGE.

PAGE 0 or 1: All BIT of the displayed PAGE become 0 or 1.

ALL 0 or 1: Each time the 0 or 1 key is pressed while pressing the GUARD key, all BIT specified by DATA LENGTH become '0' or '1'.

Next, set ② to pattern B (B LED lights) and set pattern B the same as pattern A.


However, since DATA LENGTH is common to patterns A and B, do not change it here. If it is changed, the pattern A DATA LENGTH changes also.

Two patterns (pattern A and pattern B) can be set. The number of repetitions of each pattern is controlled by ALT N A/B INPUT (rear panel). (Connected to the MP1763B)

An example when DATA LENGTH was made 128 bits is shown below.

If pattern A 0 0 0 ... 1 1 1

pattern B 1 0 1 ... 0 1 0

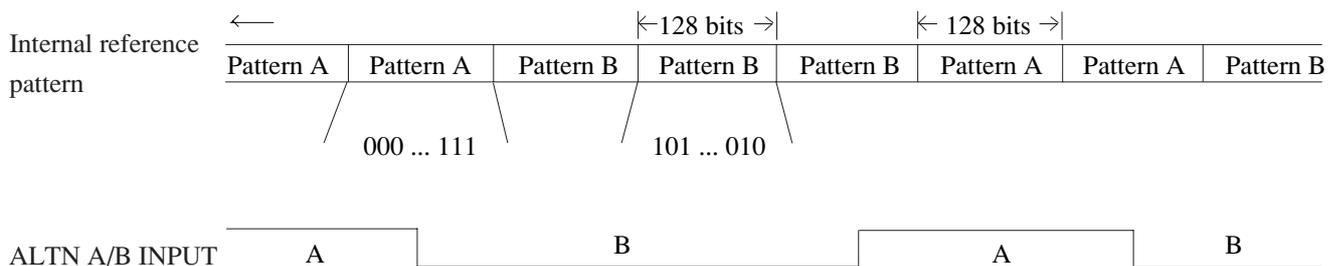


Bit 1 of Page 1 is the top of reference pattern.

Internal reference data change from pattern A to pattern B at the end of pattern A when ALT N A/B INPUT change from A to B. It is same to change from pattern B to pattern A.


Do not set pattern A and pattern B to same pattern.

SECTION 4 OPERATION

4.4.3 Data pattern setting

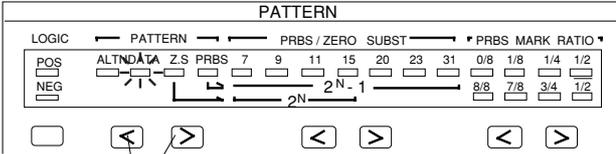

① Select DATA with the keys.

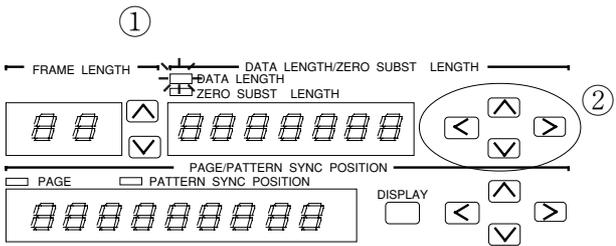

② Set DATA LENGTH with the and keys.

Select the digit to be set with the keys.


Set DATA LENGTH with the keys.

DATA LENGTH setting step

2 to 655364 : STEP 1 bit


65536 to 131012 : STEP 2 bits

Thereafter see Paragraph 1.2 Functions.

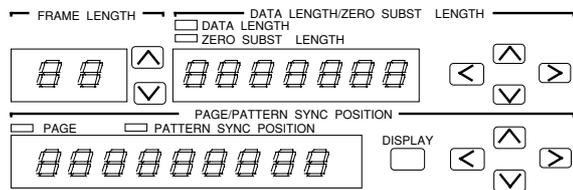

First set the page displayed at the bottom BIT display, with the set DATA LENGTH as 16 bits/page. BIT of the displayed page can be changed.

Set value: 1 to (DATA LENGTH/16)
(LENGTH is multiple of 16)
1 to INT (DATA LENGTH/16) +1
(LENGTH is not multiple of 16)

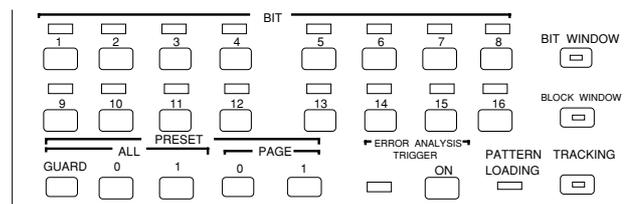

Change the BIT value with the button below the LED. When LOGIC is positive, lighting of the LED indicates High level.

When you want to change all the DATA at once, use PRESET ALL or PAGE.

PAGE 0 or 1: All BIT of the displayed PAGE become 0 or 1.


ALL 0 or 1: All BIT specified by DATA LENGTH become '0' or '1' each time the '0' or '1' key is pressed while pressing the GUARD KEY.

An arbitrary pattern is repeated as reference pattern.


When a 16 bits pattern was set:

Set pattern "0000 0101 1111 1010"


←	←		
111010	0000 0101 1111 1010	0000 0101	

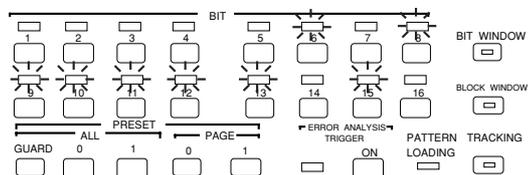


4.4.4 Zero substitution pattern setting

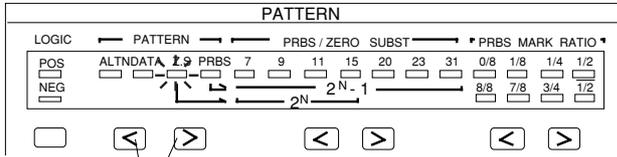

① Select Z.S. with the \leftarrow \rightarrow keys.

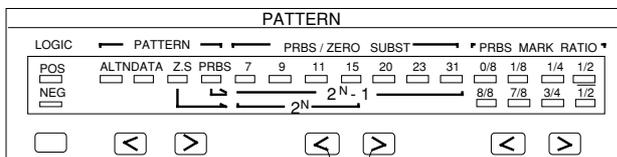

② Set 2^N pattern with the \leftarrow \rightarrow keys. (This pattern is pseudo PRBS with a 2^N period.)

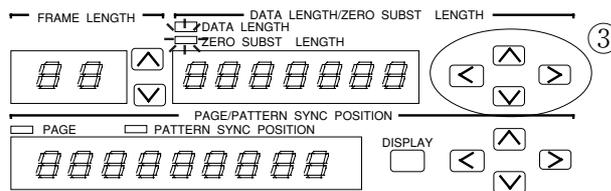

③ Set ZERO SUBSTITUTION BIT LENGTH.


Here, the pattern is substituted by a set number of bits logic '0' pattern. For a description of the substitution method, see the following.

Setting: 1 to 2^N ($N=7, 9, 11, 15$)

Pattern with the number of set bits substituted by a logic '0' pattern immediately after the maximum length of consecutive 0 bits of a pseudo PRBS (period 2^N bits: $N=7, 9, 11, 15$) with a one bit pattern of logic '1' at the end of PRBS stages 7, 9, 11, and 15. However, when the bit directly after substitution by '0' is '0', it is inverted and made '1'.


Example: Pseudo PRBS frame 7

Since the maximum length of consecutive 0 is $7-1 = 6$ bits, 0 substitution begins from the position shown below.

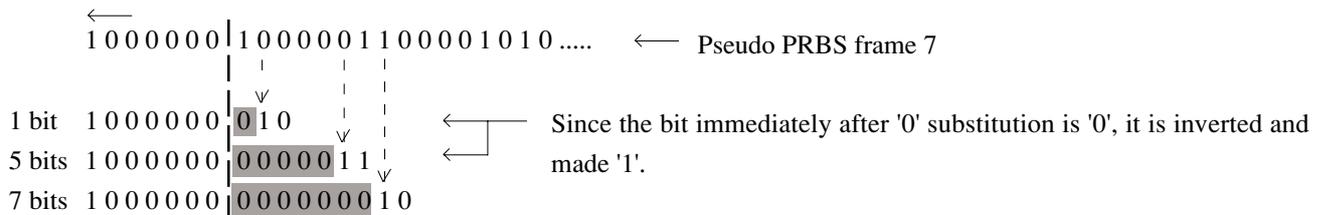


SECTION 4 OPERATION

4.4.5 Pseudo random pattern setting

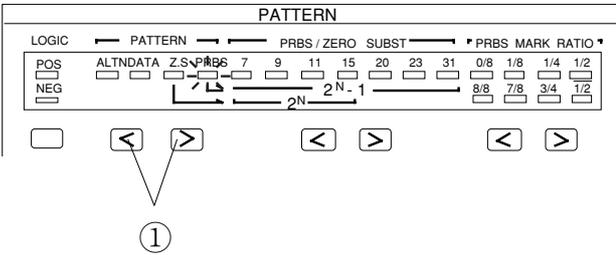

① Select PRBS with the keys.

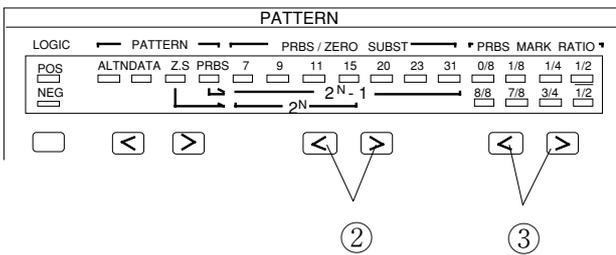

② Set the number of PRBS frames with the keys.

③ Set the PRBS mark ratio with the keys.

When LOGIC is positive, make your selection from the top row (0/8, 1/8, 1/4, 1/2).

When LOGIC is negative, make your selection from the bottom row (8/8, 7/8, 3/4, $\overline{1/2}$).


When LOGIC is changed from positive to negative when mark ratio is 1/4, the mark ratio changes to 3/4.

Pattern generated by the principle described in Paragraph 5.1 Pseudo random Pattern. When arbitrary consecutive N bits was selected in the bit array of a PRBS pattern having a period of 2^N-1 , the same bit array does not exist in one period. That is, all bit arrays can be considered other than '0' in one period.

Note: When setting pseudo random pattern, the BIT LEDs light according to the set pattern.

4.4.6 Bit window setting

This setting masks the 32 error counters in the MP1764A.

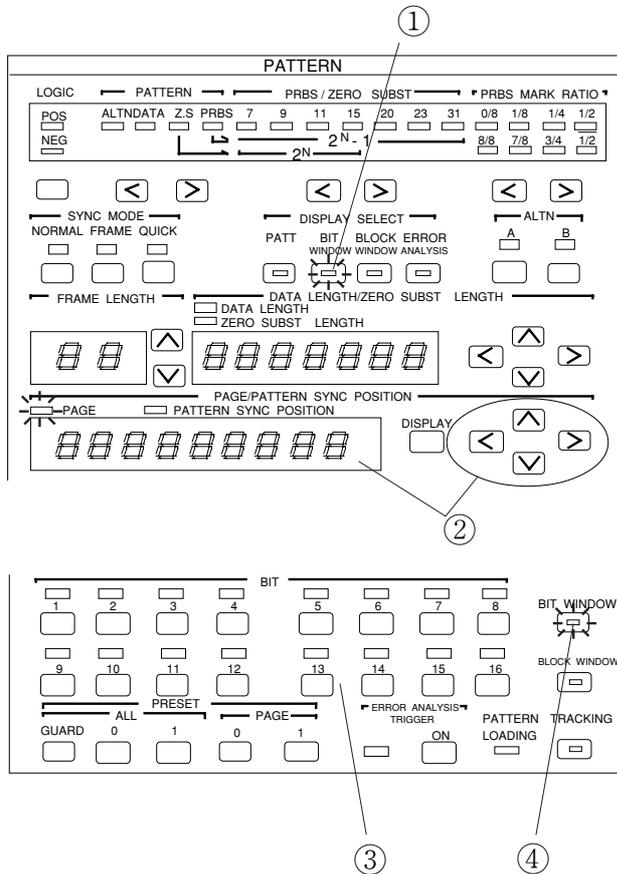


- ① Press the BIT WINDOW key of DISPLAY SELECT to light the LED inside the key.
- ② PAGE is displayed. The PAGE number is 1 to 2.
- ③ Select the channel for which the error counter is to be masked.
- ④ To actually execute the BIT WINDOW function, press the BIT WINDOW key to light the LED inside the key.


The relationship between the bits selected in ③ and the 32 error counters is as follows:

- PAGE 1, BIT 1 → Error counter number 1
- PAGE 1, BIT 2 → Error counter number 2
- ⋮
- PAGE 1, BIT 16 → Error counter number 16
- PAGE 2, BIT 1 → Error counter number 17
- PAGE 2, BIT 2 → Error counter number 18
- ⋮
- PAGE 2, BIT 16 → Error counter number 32

The bit window function masks the error counters in the MP1764A.

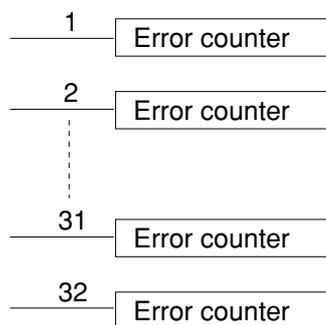

The 32 error counters detect errors in the order of set pattern bits for programmable patterns (zero substitution, DATA, and alternate). For example, for 32 bit long DATA patterns:

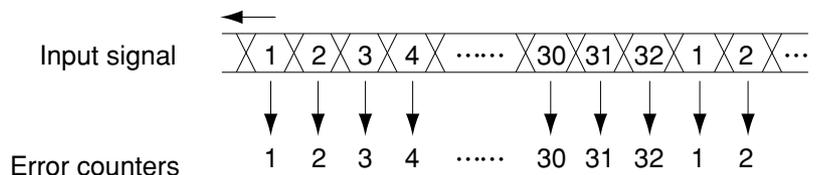


This bit window can be combined with the block window (4.4.7) to measure a 1 bit error in the measurement pattern.

SECTION 4 OPERATION

4.4.7 Block window setting

This setting masks the bits for 32 bit based pattern error measurement.

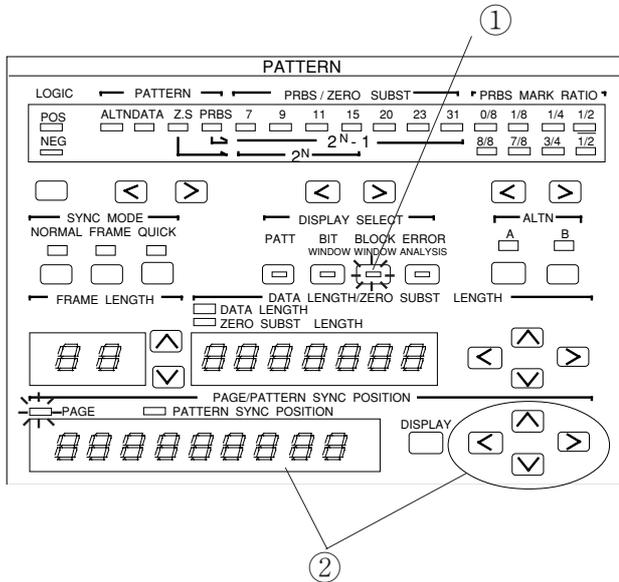


- 1 Press the BLOCK WINDOW key of DISPLAY SELECT to light the LED inside the key.

The block window is enabled for programmable patterns (zero substitution, DATA, and alternate). For DATA, the DATA length must be a multiple of 32 and the synchronization mode must not be QUICK.

- 2 Move PAGE to the pattern position where measurement masking is to be performed. The PAGE operation is the same as when PATT is selected for DISPLAY SELECT. (See Paragraphs 4.4.2 to 4.4.4)

- 3 Select a pattern mask on the BIT indicator.


When a LED is on, the bit is masked.

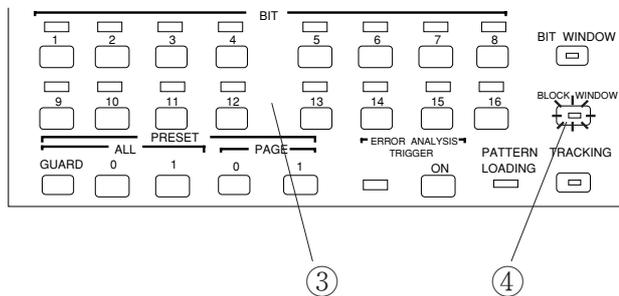

One LED of the BIT indicator indicates one bit in the pattern setting. When one key of the BIT indicator is pressed, the LEDs for all 32 bits go on or off together because the block window is turned on or off for each of the 32 bits.

- 4 To actually execute the block window function, press the BLOCK WINDOW key to light the LED inside the key.

The block window function can be used with the bit window function to measure errors on one-bit basis. Measurement can be masked by OR operation of the bit and block windows.

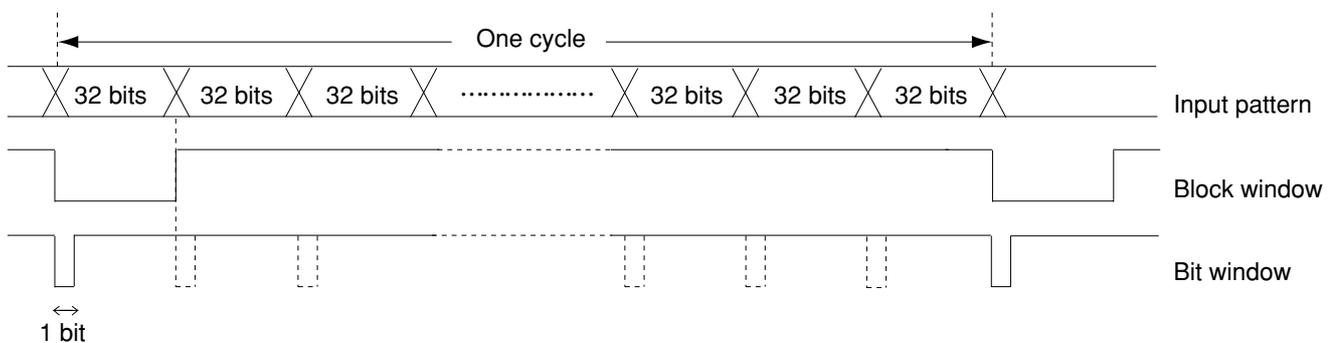

Only the high-order bit of a pattern can be measured as shown above.

4.4.8 Sync detection mode

The transmitter generated pattern and receiver pattern synchronization method is selected.


Three synchronization methods are available: NORMAL, FRAME, and QUICK. However, the following restrictions apply:

Table 4-2 Synchronization Selection Restrictions

PATTERN	SYNC MODE		
	NORMAL	FRAME	QUICK
ALTN	○	○	×
DATA	○	△*1	○
Z.S.	○	○	○
PRBS	Automatic (Internal Synchronization circuit)		

* 1 When DATA LENGTH ≥ 128 bits

Frame sync mode

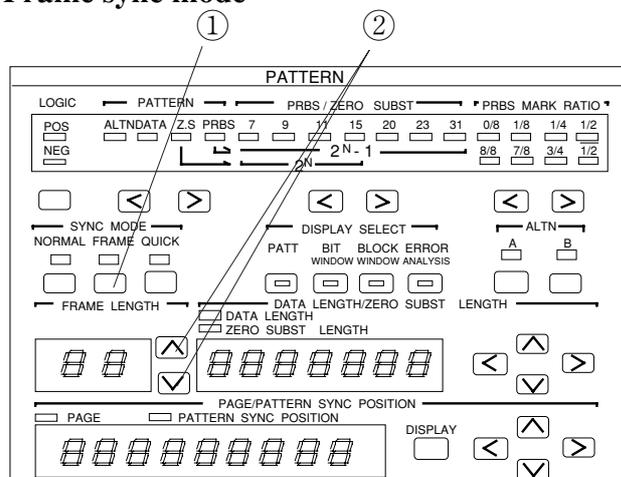

- ① Select FRAME from SYNC MODE.
- ② Set FRAME LENGTH with the keys.

Set the frame bit from the top of page 1. The set bit which represents logic '1' by orange color.

- The set value is maximum 32 bits/4 bits STEP.
- For ALTN, set the frame bit from the top of pattern A. (Pattern B is not a frame bit objective.)


Frame sync mode: Since synchronization is established by frame bit (maximum 32 bits) specified at FRAME LENGTH, when the same pattern string as frame bit exists, synchronization may take some time. The use of a special pattern at frame bit is desirable. (All '1', 'AA' repetition, etc.)

When testing with data having a long bit length, synchronization can be detected quickly by the following procedure:

- (1) Set the data.
- (2) Select the frame sync mode and make the frame length 32 bits.
- (3) Make the contents of the 32 bits a special pattern (All '1', 'AA' repetition, etc.)
- (4) Establish synchronization by automatic synchronization. (AUTO SYNC ON)
- (5) Release automatic synchronization. (AUTO SYNC OFF)
- (6) Return the changed 32-bit data to its original state.

SECTION 4 OPERATION


QUICK sync mode

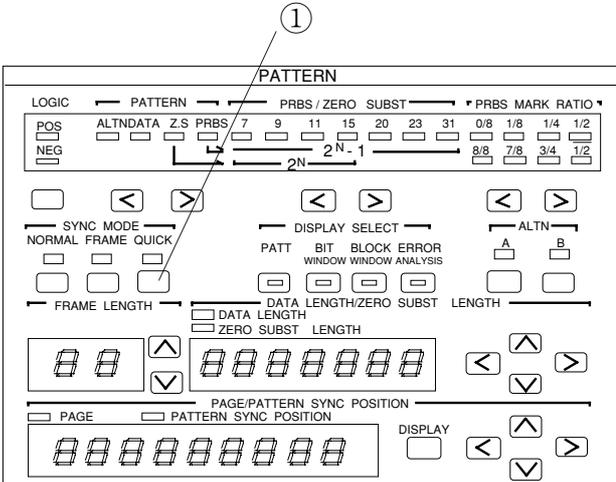

① Select QUICK from SYNC MODE.

QUICK sync mode: Method that makes error measurements by fetching data of the bit length set by DATA LENGTH to internal memory and uses the fetched pattern as the standard pattern. In this case, the pattern BIT setting is invalid.

4.4.9 Tracking

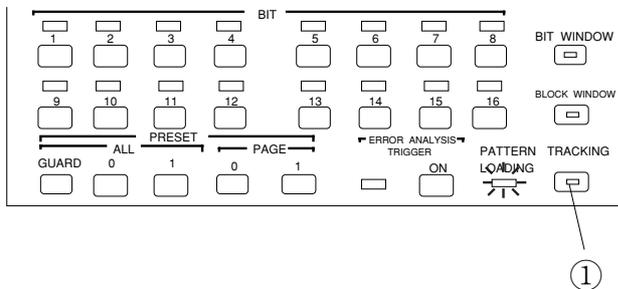

① Press the TRACKING key. The LED inside the key lights and the MP1764A enters the tracking mode.


* When tracking is performed, the MP1763B must be connected by GPIB.

When the PATTERN LOADING lamp lights, data is being read and the keys cannot be operated.

Tracking can be performed from both the receiver and the transmitter. However, one of them must be set as the master. Therefore, tracking cannot be performed simultaneously from both the receiver and the transmitter.

When performing tracking, set 'SYSTEM CONTROL' of the DIP switch on the rear panel of the master unit to 'ON'. (Set 'SYSTEM CONTROL' of the controlled unit to 'OFF'.)

Set GPIB ADDRESS of the controlled unit to master unit GPIB ADDRESS + 2.




Each time the settings of the master unit (receiver or transmitter) are changed in the tracking ON state, the settings of the transmitter (or receiver) are changed. Therefore, each time a master key is operated, an unavailable state is generated. (Especially, when the program bit length is long, an unavailable state of several tens of seconds is generated.) To prevent this, when changing the master unit settings, set tracking to OFF.

SECTION 4 OPERATION

4.4.10 Error analysis (Option 01)

At error detection, 256 bits of data are memorized and the error and the data before and after it can be checked.

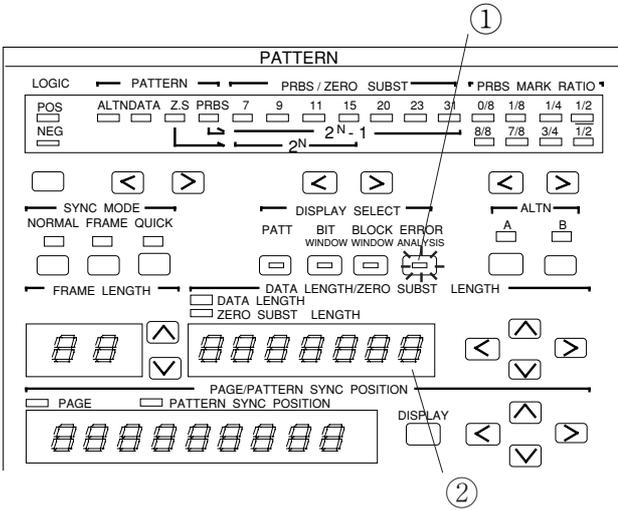


① Press the ERROR ANALYSIS key. The LED inside the key lights.

② Change the display page for the ERROR ANALYSIS DATA.


Sixteen pages, including the pattern that generated an error, can be set.

Pages 9 and 10 display the BIT that generated an error and became the trigger.

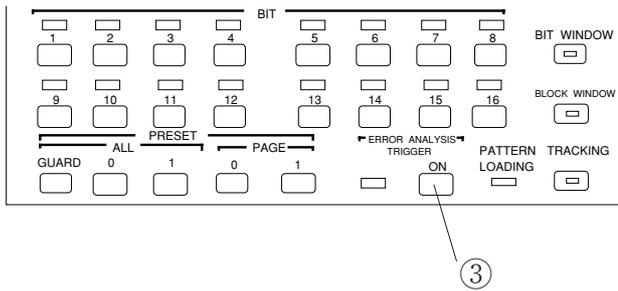

③ Set ERROR ANALYSIS TRIGGER to ON.

Result Display

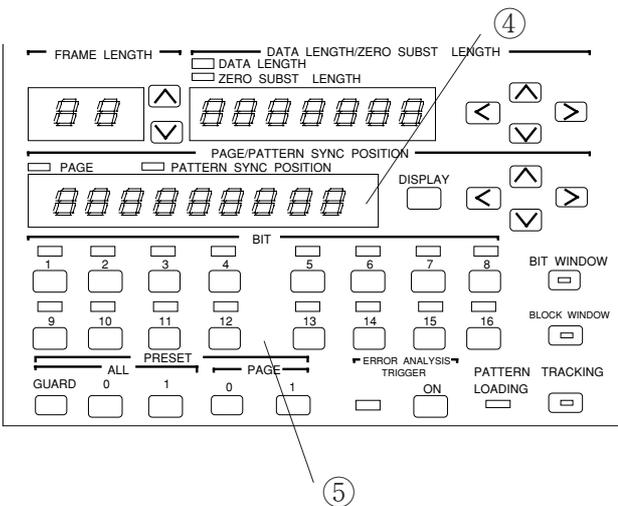

④ The display page is shown.

Page position shows the pattern setting and display page position.


⑤ The error is indicated by a red or orange LED. (See Table 4-3.)

Table 4-3

Receive data	Reference	LED	
0	0	OFF	Normal
1	1	Green	Normal
0	1	Red	Insertion error
1	0	Orange	Omission error

* When performing error analysis using the PRBS $2^{31}-1$ pattern, a few seconds after synchronization is established before starting analysis.

4.5 Error Measurement

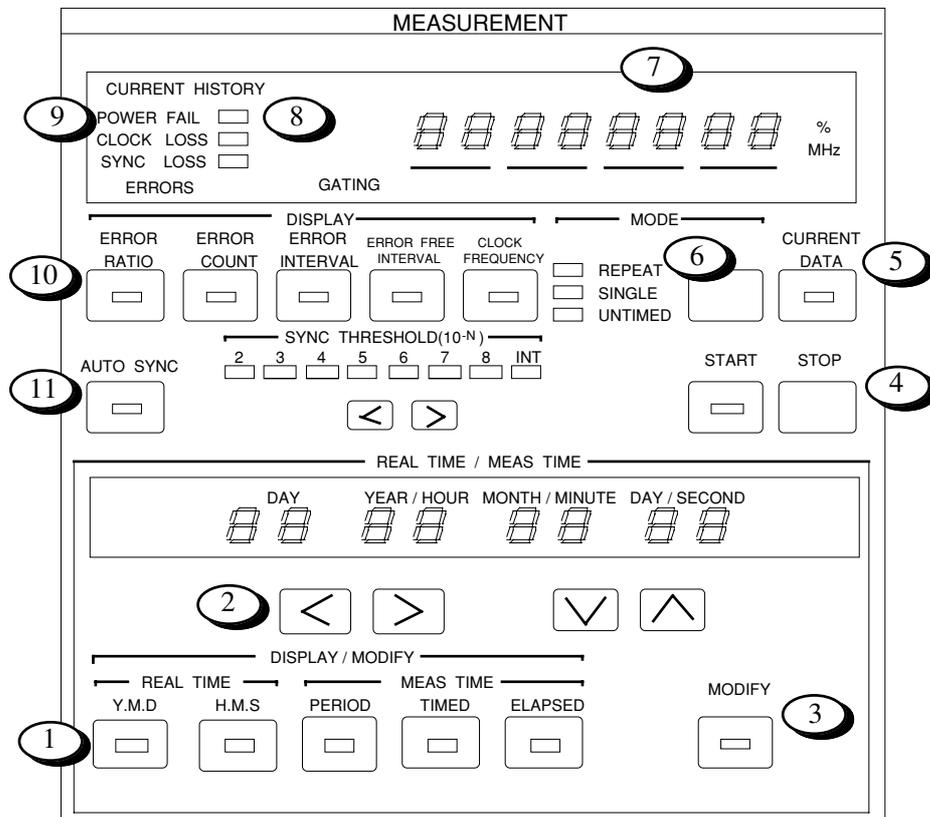

1 DISPLAY/MODIFY key

REAL TIME

Y.H.D. Press to set or display the date. When the lamp inside the key lights, the date is displayed on the display.

H.M.S. Press to set or display the time., When the lamp inside the key lights, the time is displayed on the display.

MEAS TIME

PERIOD Press to set or display the measurement time (gating time). When the LED inside the key lights, the measurement time (gating time) is displayed on the display.

TIME Press to display the remaining measurement time. When the LED inside the key lights, the remaining time is displayed on the display. Cannot be selected when the measurement mode is UNTIMED.

ELAPSED Press to display the elapsed measurement time. When the LED inside the key lights, the elapsed time is displayed on the display.

SECTION 4 OPERATION

- 2**     keys

  keys Select the item to be set when setting REAL TIME. The selected item blinks.

  keys Used when raising and lowering the set value.
- 3** MODIFY key

Pressed when changing the REAL TIME or MEAS TIME setting. When the LED inside the key lights, the set value can be changed.
- 4** START / STOP keys

Start and stop measurement. During measurement, the LED inside the START key remains lit.
- 5** CURRENT DATA key

Turns the data display on and off during measurement. When the LED inside the key is lit, the current measurement data is displayed.
- 6** Measurement mode selection keys

Select the measurement mode from among REPEAT, SINGLE, and UNTIMED.

REPEAT : Repeated measurement
 SINGLE : One measurement
 UNTIMED : Manual measurement (accumulative measurement)
- 7** Display

Displays the measured result. The display contents are selected with **10**.
- 8** HISTORY key

Displays the past state. (Displays the result of the last measurement.)

POWER FAIL : Lamp that shows that the power dipped or failed. (History lamp only)
 CLOCK LOSS : Display and lamp that show that the clock pulses were lost.
 SYNC LOSS : Display and lamp that show that synchronization was lost.
- 9** CURRENT lamp


Displays the current measurement state.
- 10** DISPLAY display switching keys

Select the item displayed on the display. The item at which the internal LED is lit is displayed.


ERROR RATIO : Displays the error ratio.
 ERROR COUNT : Displays the number of errors.
 ERROR INTERVAL : Displays the number of error intervals (EI).
 ERROR FREE INTERVAL : Displays the number of error free intervals ratio(EFI).
 CLOCK FREQUENCY : Displays the clock frequency.
- 11** AUTO SYNC key

Turns the pattern automatic synchronization function on and off.


4.5.1 ERROR RATIO measurement

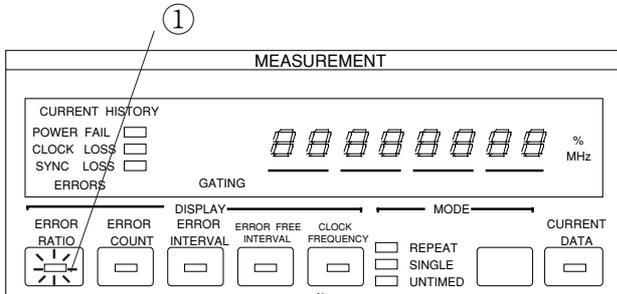


① Press the ERROR RATIO key. The LED inside the key lights and the ERROR RATIO measured result is displayed at DISPLAY.

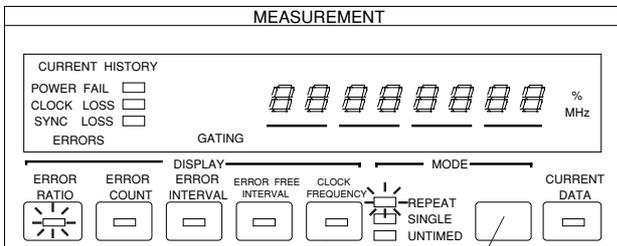

② Press the MODE key and select REPEAT. (See 4.5.7.) When REPEAT is selected, the DISPLAY display value is updated at each MEAS TIME set value.

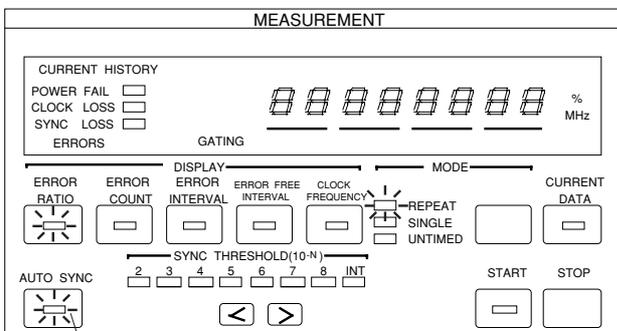


③ Set AUTO SYNC to ON. (Internal LED lights) During normal measurement, the AUTO SYNC key is usually left in the ON position. (See 4.5.10.).

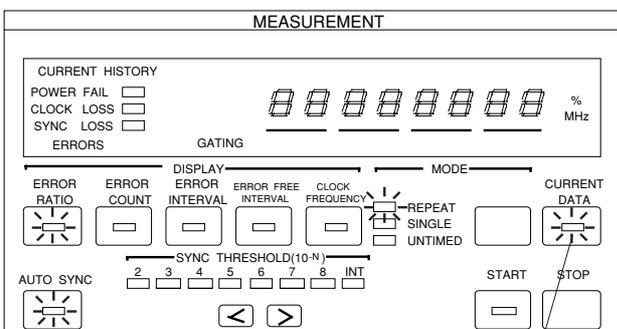

④ When you want to display the result during measurement, press the CURRENT DATA key. The LED inside the key lights. When CURRENT DATA is ON, the current measured result is displayed at each measurement time. (See 4.5.11.)

SECTION 4 OPERATION


4.5.2 ERROR COUNT

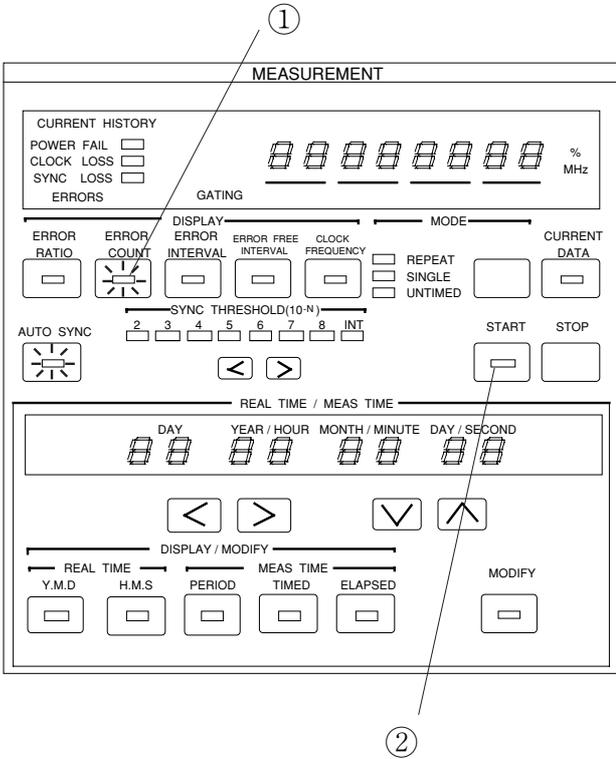

- ① Press the ERROR COUNT key. The LED inside the key lights and the ERROR COUNT measured result is displayed at DISPLAY.
- ② Set MODE (Paragraph 4.5.2) and MEAS TIME (Paragraph 4.5.11) and start measurement by pressing the START key.

In the AUTO SYNC OFF state, synchronization is not established. Therefore, always leave the AUTO SYNC key in the ON position.


4.5.3 ERROR INTERVAL

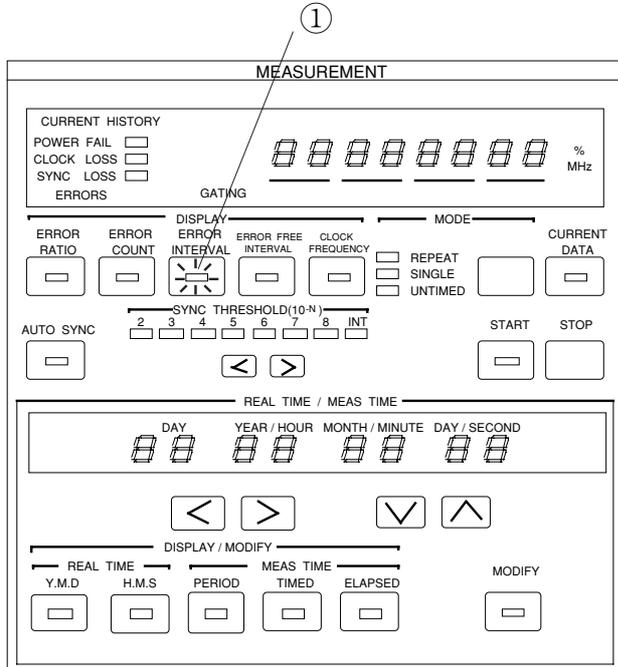

① Press the ERROR INTERVAL key. The LED inside the key lights.

② Select the measurement mode. (See 4.5.1.)

③ Set MEAS TIME. (See 4.5.11.)

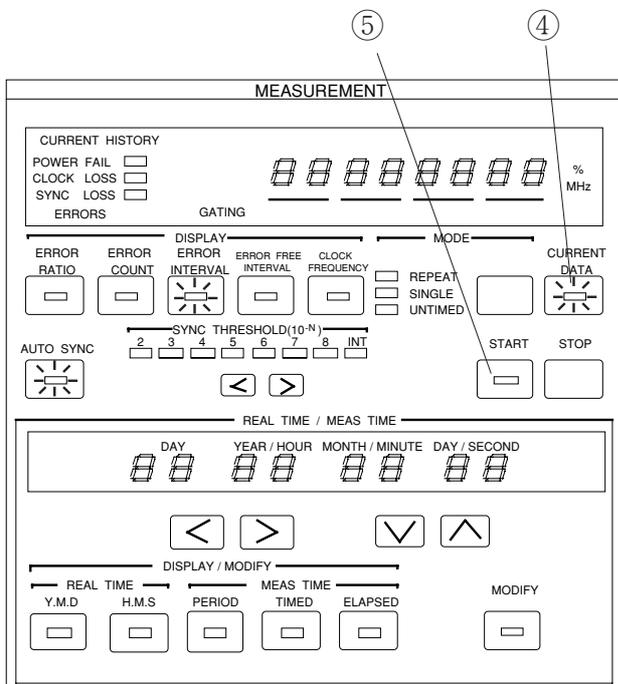


④ When an intermediate measured result is necessary, press the CURRENT DATA key. The LED inside the key lights. (See 4.5.9.)

⑤ Start measurement by pressing the START key.

* During measurement, always leave the AUTO SYNC key in the ON position. (See 4.5.10.)

SECTION 4 OPERATION


4.5.4 ERROR FREE INTERVAL

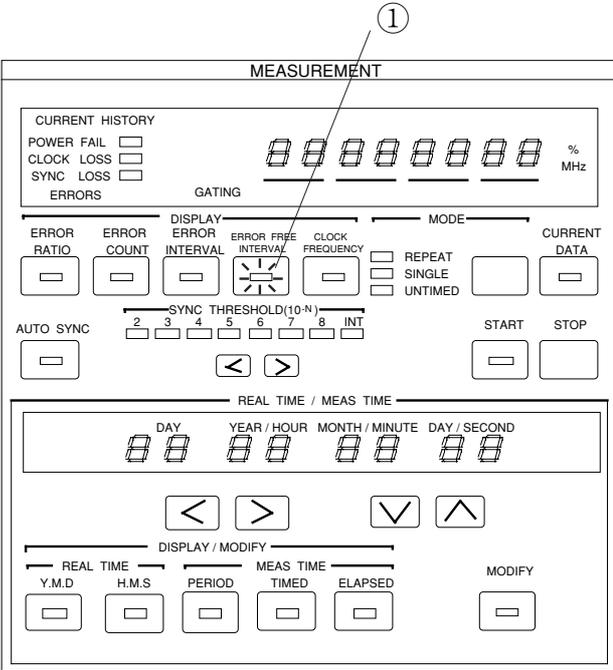

① Press the ERROR FREE INTERVAL key. The LED inside the key lights.

② Select the measurement mode. (See 4.5.1.)

③ Set MEAS TIME. (See 4.5.11.)

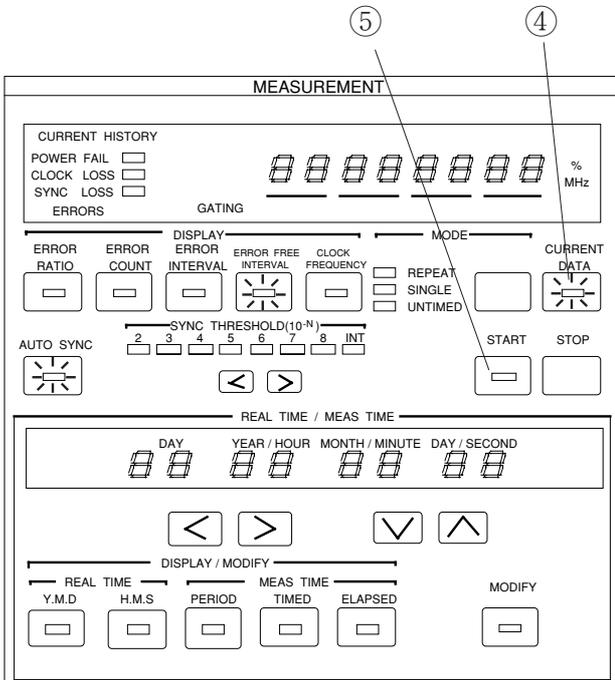


④ When an intermediate measured result is necessary, press the CURRENT DATA key. The LED inside the key lights. (See 4.5.9.)

⑤ Start measurement by pressing the START key.

* During measurement, always leave the AUTO SYNC key in the ON position. (See 4.5.10.)


4.5.5 CLOCK FREQUENCY

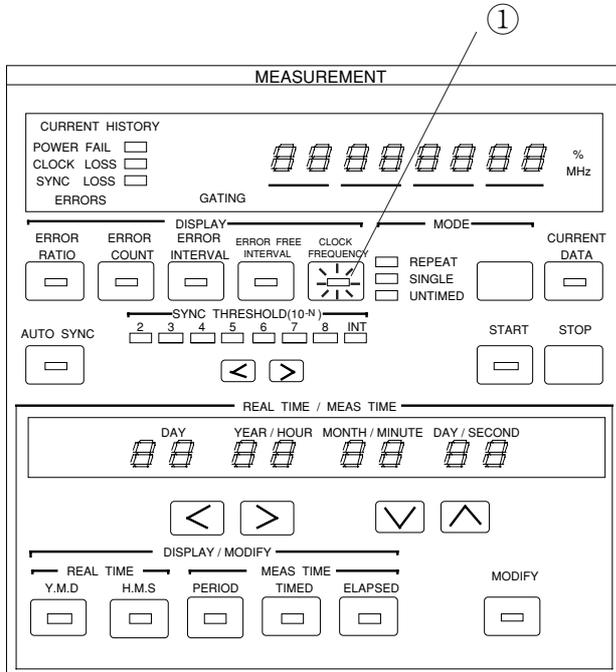

- ① Press the CLOCK FREQUENCY key. The LED inside the key lights.
- ② For SYNC LOSS, CLOCK FREQUENCY is not displayed. In this case, make measurements with the AUTO SYNC key set to OFF. If the clock pulse is input normally, CLOCK FREQ. is correctly displayed.

SECTION 4 OPERATION

4.5.6 DISPLAY display

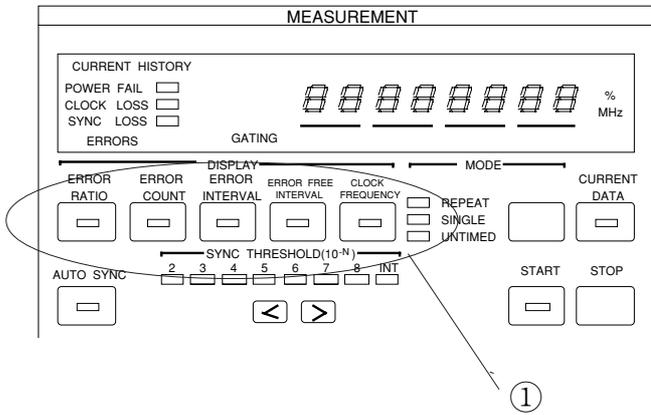

① Select the item to be displayed at DISPLAY from among error ratio, error count, error intervals, error free intervals, and clock frequency.

Press the key of the item you want to display. The LED inside the key lights.

DISPLAY display of each item is shown below.

(1) Error ratio

0.0000-16 to 1.0000E-0

(2) Error count

△△△△△△△0 to △9999999
1.0000E07 to 9.9999E-16

(3) Error intervals (EI) count

△△△△△△△0 to △9999999

(4) Error free intervals (EFI) ratio


△△△0.0000 to △100.000 (% units display lights)

(5) Clock frequency

△△△50.000 to 12500.000 (MHz units display lights)

Note: During sync loss, '-' is displayed at all digits. If the AUTO SYNC key is set to OFF at this time, the clock frequency is displayed.

4.5.7 Measurement mode selection

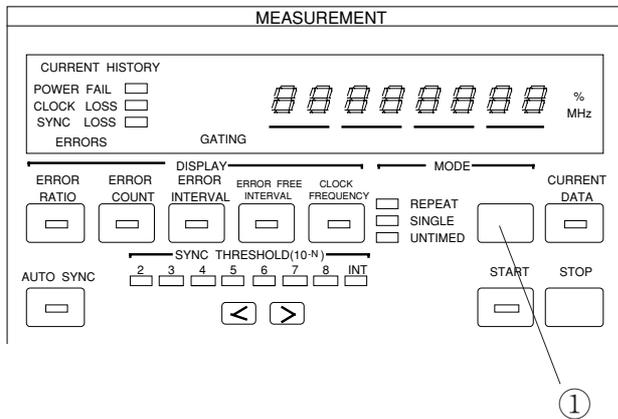

① Press the MODE key and select the measurement mode. The measurement mode changes in REPEAT → SINGLE → UNTIMED → REPEAT... order and the LED of the selected item lights.

When selecting REPEAT or SINGLE, set the measurement time in accordance with Paragraph 4.5.11.

The measurement modes are defined below.

(1) REPEAT mode

Unit measurement is repeated continuously during the set measurement time.


(2) SINGLE mode

Unit measurement is performed once during the set measuring time.

(3) UNTIMED mode

After the START key is pressed, measurement is performed continuously until the STOP key is pressed.

4.5.8 Measurement start/stop

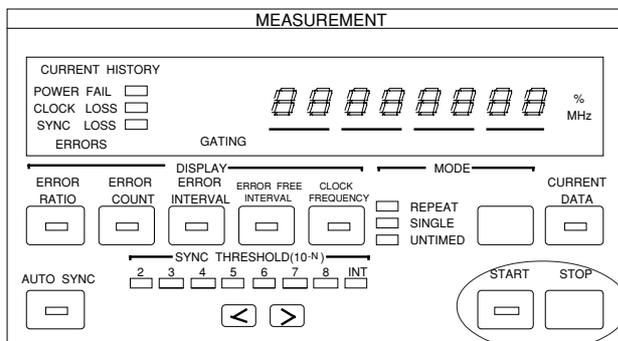

When the START key is pressed, the start lamp lights and measurement starts in accordance with the measurement mode.


When the STOP key is pressed, the START lamp goes off and measurement stops. When the START key is pressed during measurement, measurement is restarted.

In the SINGLE mode, when the measurement time ends before the STOP key is pressed, the START lamp goes off automatically and measurement stops.

SECTION 4 OPERATION

4.5.9 Current data function

The current data function can display intermediate measured results at the specified cycle time (0.1, 0.2 secs). There are two intermediate measured result calculation modes: PROGRESSIVE mode and IMMEDIATE mode. In the PROGRESSIVE mode, the result accumulated from the start of measurement is displayed. In the IMMEDIATE mode, the instantaneous result of each cycle time is displayed. An example of display of the measured result for 2 seconds measurement time and 0.2 second cycle time is shown in Fig. 4-3.

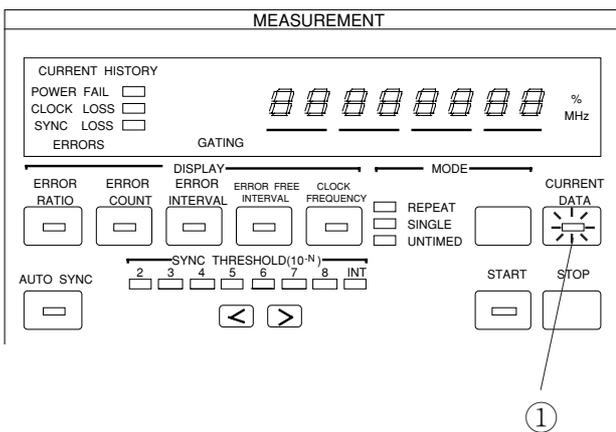

① Press the CURRENT DATA key. The LED inside the key lights.

② Set rear panel FUNCTION1 SW6. (Calculation mode setting)

SW6

0: PROGRESSIVE mode

1: IMMEDIATE mode

③ Set rear panel FUNCTION2 SW9. (Cycle time setting)

SW9 Cycle time

0 0.1 sec

1 0.2 sec

The measurement time and calculation mode have the following relationship:


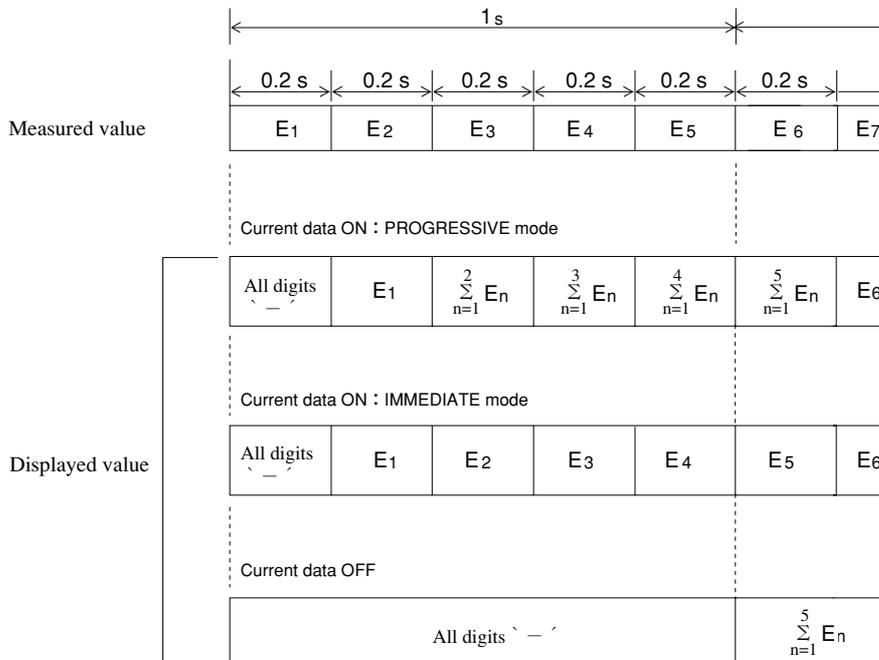


Fig. 4-3

4.5.10 AUTO SYNC function

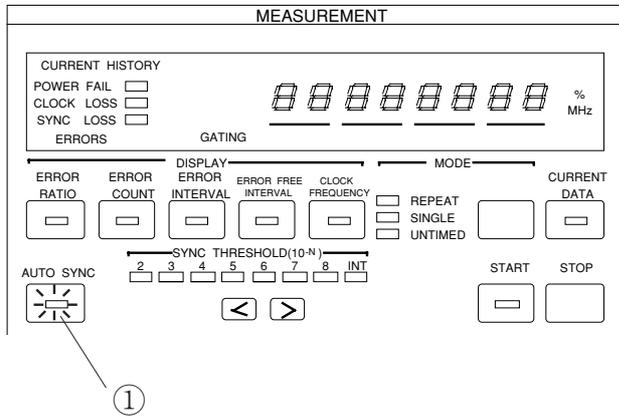

- ① In normal measurement, the AUTO SYNC function is turned on and input pattern and comparison pattern synchronization is established automatically. To turn on the AUTO SYNC function, press the AUTO SYNC key. The lamp inside the key lights.

The AUTO SYNC function has a normal mode, a frame mode and a quick mode. The monitor pattern during sync loss is different in the normal mode and the frame mode. Whereas the monitor pattern in the normal mode is all patterns, the monitor pattern in the frame mode is only a specific pattern of from 4 to 32 bits (hereinafter referred to as "frame bits").

The frame mode can be set only when one period is a programmable pattern of at least 128 bits. The synchronization pull-in time can be made shorter than the normal pattern by monitoring only the frame bits.

- ② To set the AUTO SYNC function to the frame mode, select frame at SYNC MODE. The lamp lights and the frame sync function is turned on. For a description of frame bit length and frame bit setting, see 5.2.4 Frame sync function setting.

When number of errors is large

Ordinary, the AUTO SYNC function is left on during measurement. However, when the number of errors extremely large (larger than the sync pull-in value) and synchronization cannot be established, the pull-in value can be set manually. Moreover, once synchronization has been established by AUTO SYNC function, error measurements can be made, even if the number of errors is extremely large, by tuning off the AUTO SYNC function. However, when the frequency is changed, measurement may become impossible.

When SYNC THRESHOLD is INT

Sync pull-in state or sync loss state judgment is performed by sync threshold value. In the sync pull-in state, when the error ratio exceeds the sync loss threshold value, the sync loss state is judged. In the sync loss state, when the error ratio drops below the sync recovery threshold value, the sync pull-in state is judged. When the error ratio always exceeds the sync loss threshold value, pattern synchronization is not established and measurements cannot be made. However, when the error ratio is smaller than the sync loss threshold value, pattern synchronization is established by setting the AUTO SYNC to ON. Thereafter, if the AUTO SYNC key is set to OFF and the pattern sync circuit is locked, measurements can be made even if the error ratio exceeds the sync loss threshold value.

As SYNC THRESHOLD, INT or either of 10^{-2} to 10^{-8} can be selected. Refer to Fig. 4-4-1 for INT, and refer to Fig. 4-4-2 for either of 10^{-2} to 10^{-8} .

Example: PRBS threshold value when SYNC THRESHOLD made 10^{-5} (See Table 4-4-2.)
 Sync pull-in threshold value
 1.56×10^{-5}
 Sync loss threshold value
 5×10^{-5}

SECTION 4 OPERATION

Table 4-4-1 Sync Threshold Values (At INT)

Mode	Pattern	Data length	Sync threshold value Error ratio= $\left(\frac{\text{Error count}}{\text{Clock count}}\right)$	
			Sync pull-in state→sync loss state When normal	Sync loss state→sync pull-in state (When abnormal)
Normal	PRBS	2^{N-1} (N=7, 9, 11, 15, 20, 23, 31)	$\frac{(128) \times 2,000}{(2,048) \times 2,500} = \frac{1}{20} = 5 \times 10^{-2}$	$\frac{(64)}{(2,048) \times 2} = \frac{1}{64} = 1.56 \times 10^{-2}$
	ALTN/DATA /Z.S.	2~16	$\frac{(128) \times 2,000}{(2,048) \times 2,500} = \frac{1}{20} = 5 \times 10^{-2}$	$\frac{(64)}{(2,048) \times 2} = \frac{1}{64} = 1.56 \times 10^{-2}$
		17~160	$\frac{(128) \times 200}{(2,048) \times 2,500} = \frac{1}{200} = 5 \times 10^{-3}$	$\frac{(64)}{(2,048) \times 20} = \frac{1}{640} = 1.56 \times 10^{-3}$
		161~1,600	$\frac{(128) \times 20}{(2,048) \times 2,500} = \frac{1}{2,000} = 5 \times 10^{-4}$	$\frac{(64)}{(2,048) \times 200} = \frac{1}{6400} = 1.56 \times 10^{-4}$
		1,601~16,000	$\frac{(128) \times 2}{(2,048) \times 2,500} = \frac{1}{20,000} = 5 \times 10^{-5}$	$\frac{(64)}{(2,048) \times 2,000} = \frac{1}{64,000} = 1.56 \times 10^{-5}$
		16,001~80,000	$\frac{(128) \times 2}{(2,048) \times 12,500} = \frac{1}{100,000} = 1 \times 10^{-5}$	$\frac{(64)}{(2,048) \times 5,000} = \frac{1}{160,000} = 6.25 \times 10^{-6}$
		20,001~160,000	$\frac{(128) \times 2}{(2,048) \times 25,000} = \frac{1}{200,000} = 5 \times 10^{-6}$	$\frac{(64)}{(2,048) \times 10,000} = \frac{1}{320,000} = 3.13 \times 10^{-6}$
		160,001~320,000	$\frac{(128) \times 2}{(2,048) \times 500,000} = \frac{1}{400,000} = 2.5 \times 10^{-6}$	$\frac{(64)}{(2,048) \times 20,000} = \frac{1}{640,000} = 1.56 \times 10^{-6}$
		320,001~524,288	$\frac{(128) \times 2}{(2,048) \times 2^{16}} = \frac{1}{524,288} = 1.9 \times 10^{-6}$	$\frac{(64)}{(2,048) \times 40,000} = \frac{1}{1,280,000} = 7.81 \times 10^{-7}$
		524,289~1,048,576	$\frac{(128) \times 2}{(2,048) \times 2^{17}} = \frac{1}{1,048,576} = 9.54 \times 10^{-7}$	$\frac{(64)}{(2,048) \times 80,000} = \frac{1}{2,560,000} = 3.91 \times 10^{-7}$
		1,648,577~2,097,152	$\frac{(128) \times 2}{(2,048) \times 2^{18}} = \frac{1}{2,097,152} = 4.77 \times 10^{-7}$	$\frac{(64)}{(2,048) \times 160,000} = \frac{1}{5,120,000} = 1.96 \times 10^{-7}$
		2,097,153~4,194,304	$\frac{(128) \times 2}{(2,048) \times 2^{19}} = \frac{1}{4,194,304} = 2.38 \times 10^{-7}$	$\frac{(64)}{(2,048) \times 320,000} = \frac{1}{10,240,000} = 9.80 \times 10^{-8}$
		4,194,305~8,388,608	$\frac{(128) \times 2}{(2,048) \times 2^{20}} = \frac{1}{8,388,608} = 1.19 \times 10^{-7}$	$\frac{(64)}{(2,048) \times 640,000} = \frac{1}{20,480,000} = 4.90 \times 10^{-8}$
		Frame /quick	ALTN/DATA /Z.S.	128~5,120
5,121~10,240	$\frac{(128) \times 100}{(2,048) \times 68,750} = \frac{1}{11,000} = 9.1 \times 10^{-5}$			
10,241~51,200	$\frac{(128) \times 100}{(2,048) \times 10 \times 32,500} = \frac{1}{52,000} = 1.9 \times 10^{-5}$			
51,201~102,400	$\frac{(128) \times 100}{(2,048) \times 20 \times 34,375} = \frac{1}{110,000} = 9.1 \times 10^{-6}$			
102,401~204,800	$\frac{(128) \times 100}{(2,048) \times 50 \times 26,250} = \frac{1}{210,000} = 4.8 \times 10^{-6}$			
204,801~307,200	$\frac{(128) \times 100}{(2,048) \times 50 \times 38,750} = \frac{1}{310,000} = 3.2 \times 10^{-6}$			
307,201~409,600	$\frac{(128) \times 100}{(2,048) \times 50 \times 51,250} = \frac{1}{410,000} = 2.4 \times 10^{-6}$			
409,601~524,288	$\frac{(128) \times 100}{(2,048) \times 50 \times 32,768} = \frac{1}{530,000} = 1.9 \times 10^{-6}$			
524,289~1,048,576	$\frac{(128) \times 100}{(2,048) \times 687,500} = \frac{1}{110,000} = 9.1 \times 10^{-7}$			
1,048,577~2,097,152	$\frac{(128) \times 100}{(2,048) \times 13,125,000} = \frac{1}{2,100,000} = 4.8 \times 10^{-7}$			
2,097,153~4,194,304	$\frac{(128) \times 100}{(2,048) \times 26,250,000} = \frac{1}{4,200,000} = 2.4 \times 10^{-7}$			
4,194,305~8,388,608	$\frac{(128) \times 100}{(2,048) \times 52,500,000} = \frac{1}{8,400,000} = 1.2 \times 10^{-7}$			

Note: For ALTN pattern, the maximum length is 4194304 bits and the Z.S. pattern data length is 2^N (N=7, 9, 11, 15) bits and the threshold value becomes the threshold value of the corresponding data length.

Example) For 2^7 , the data length is $2^7=128$ and corresponds to a value of 17 to 160.

Table 4-4-2 Sync Threshold Values (At 10^{-2} to 10^{-8})


The Sync Threshold values are independent from the Pattern and Data Length.

SYNC THRESHOLD	Sync threshold value Error ratio = $\left(\frac{\text{Error count}}{\text{Clock count}} \right)$	
	Sync pull-in state → sync loss state When normal	Sync loss state → sync pull-in state (When abnormal)
10^{-2}	$\frac{(128) \times 2,000}{(2,048) \times 2,500} = 5 \times 10^{-2}$	$\frac{(64)}{(2,048) \times 2} = 1.56 \times 10^{-2}$
10^{-3}	$\frac{(128) \times 2,000}{(2,048) \times 25,000} = 5 \times 10^{-3}$	$\frac{(64)}{(2,048) \times 20} = 1.56 \times 10^{-3}$
10^{-4}	$\frac{(128) \times 2,000}{(2,048) \times 250,000} = 5 \times 10^{-4}$	$\frac{(64)}{(2,048) \times 200} = 1.56 \times 10^{-4}$
10^{-5}	$\frac{(128) \times 2,000}{(2,048) \times 2,500,000} = 5 \times 10^{-5}$	$\frac{(64)}{(2,048) \times 2,000} = 1.56 \times 10^{-5}$
10^{-6}	$\frac{(128) \times 2,000}{(2,048) \times 25,000,000} = 5 \times 10^{-6}$	$\frac{(64)}{(2,048) \times 20,000} = 1.56 \times 10^{-6}$
10^{-7}	$\frac{(128) \times 200}{(2,048) \times 25,000,000} = 5 \times 10^{-7}$	$\frac{(64)}{(2,048) \times 200,000} = 1.56 \times 10^{-7}$
10^{-8}	$\frac{(128) \times 20}{(2,048) \times 25,000,000} = 5 \times 10^{-8}$	$\frac{(64)}{(2,048) \times 2,000,000} = 1.56 \times 10^{-8}$

SECTION 4 OPERATION

4.5.11 Measurement time setting

This setting sets the measurement time in the REPEAT and SINGLE measurement modes.

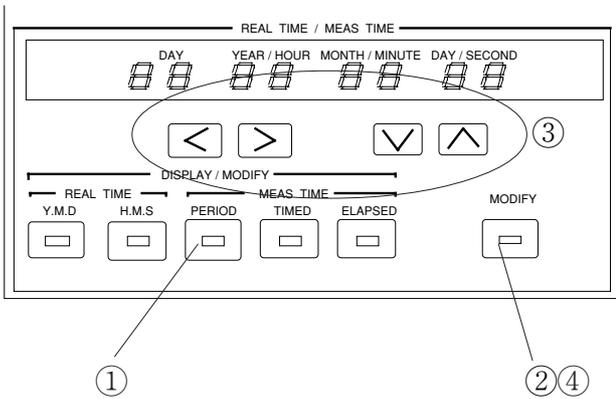

- ① Press the PERIOD key. The currently set measurement time is displayed at DISPLAY.
- ② Press the MODIFY key. The figures on DISPLAY that can be changed begin to blink.
- ③ Set the DAY, HOUR, MINUTE, and SECOND values with the \leftarrow \rightarrow and \uparrow \downarrow keys.
- ④ Press the MODIFY key again. The DISPLAY stops blinking and the measurement time is set. Check if the LED inside the MODIFY key is off.

* When the set value is 00 day 00 hour 00 minute 00 second, the MODIFY key is not turned off.

Measurements are made at the initially set time even if a power failure, clock loss, or sync loss alarm is generated during measurement.


The measurement time and minimum measurable error ratio have the following relationship:

$$\text{Minimum error ratio} = \frac{1}{\text{Measurement time (sec)} \times \text{frequency (Hz)}}$$

Example: When the measurement time is 10 seconds and the frequency is 10 GHz, the minimum error ratio is 1×10^{-11} .

4.5.12 Real time setting


This setting sets the internal calendar clock.

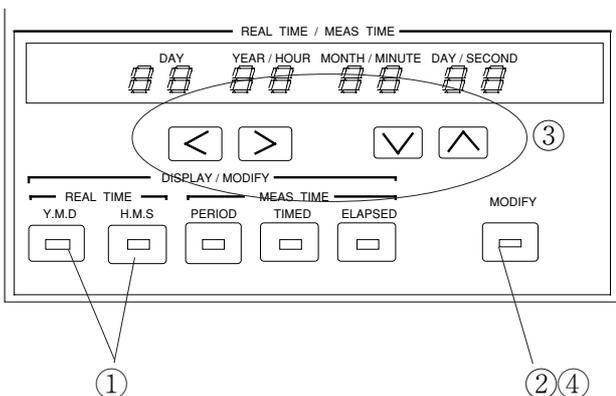

- ① Press the Y.M.D or H.M.S key. The date or time is displayed at DISPLAY. Display the item to be changed.
- ② Press the MODIFY key. The figures on DISPLAY that can be changed begin to blink.
- ③ Change the date or time with the \leftarrow \rightarrow and \uparrow \downarrow keys.
- ④ Press the MODIFY key again. The DISPLAY stops blinking and setting is complete.

* When the set value is an impossible value, the MODIFY key is not turned off.

4.5.13 Error lamp and alarm lamps

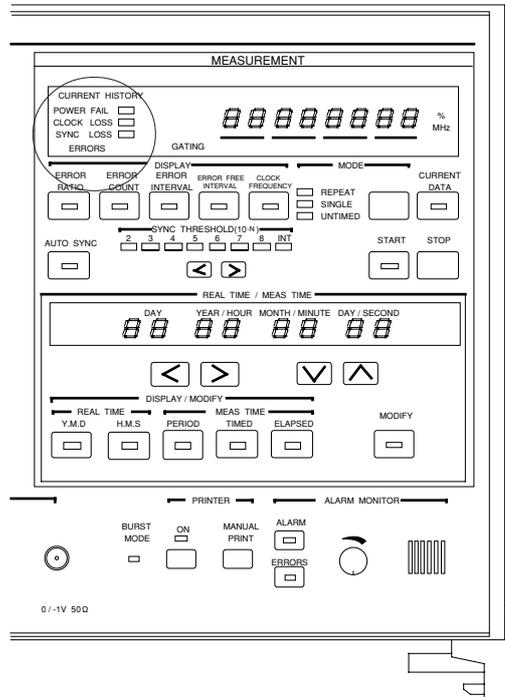

(1) Error lamp

This lamp indicates that an error was generated.

- ON condition: When error generated
- OFF condition: When there are no errors and at clock loss and sync loss

(2) Alarm lamps

The alarm lamps are made up of a HISTORY lamp (orange, small) that displays the past state and a realtime lamp (orange, large) that displays the current state.

(a) POWER FAIL lamp (HISTORY lamp only)

This lamp indicates generation of a power dip or power failure alarm.

- ON condition HISTORY lamp: After power is recovered when a power dip or power failure occurred during measurement.
- OFF condition HISTORY lamp: At the start of measurement.

(b) CLOCK LOSS lamps

These lamps indicate that a clock loss alarm was generated.

- ON condition HISTORY lamp: When clock loss alarm generated during measurement.
Realtime lamp : When clock loss alarm generated.
- OFF condition HISTORY lamp: At start of measurement.
Realtime lamp : When clock signal recovered.

(c) SYNC LOSS lamps

These lamps indicate that a sync loss alarm was generated.

- ON condition HISTORY lamp: When sync loss alarm generated during measurement.
Realtime lamp : When sync loss alarm generated.
- OFF condition HISTORY lamp: At start of measurement.
Realtime lamp : When synchronization recovered and when clock loss alarm generated and when the AUTO SYNC key is OFF.

SECTION 4 OPERATION

4.5.14 Error detection mode setting

Errors are detected by comparing each bit of the input pattern to an internally generated pattern. The error detection mode has three kinds of errors: total error, insertion error, and omission error. The kind of error is selected by rear panel FUNCTION1 SW7 and SW8 as shown below.

SW7	SW8	Error
0	0	Total error
0	1	Insertion error
1	0	Omission error
1	1	Total error

In the insertion error mode, the pattern is detected only as an error of BIT that changed from "0" to "1". In the omission error mode, the pattern is detected as an error of only BIT that changed from "1" to "0". In the total error mode, all errors are detected.

In Fig. 4-4, the pattern logic was set to positive logic. When the pattern logic was set to negative logic, (d) becomes an omission error and (e) becomes an insertion error.


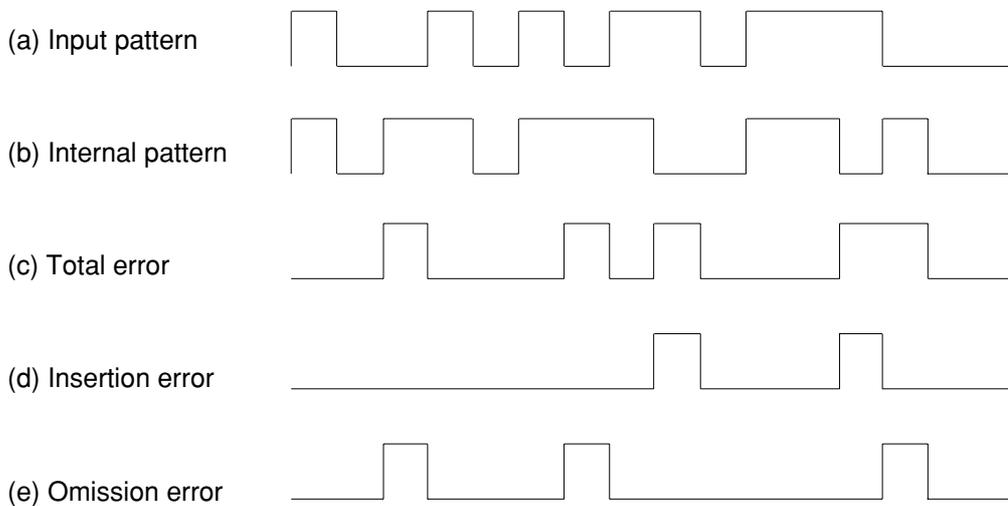


Fig. 4-4 Error Detection Mode


4.6 Memory (Floppy Disk)

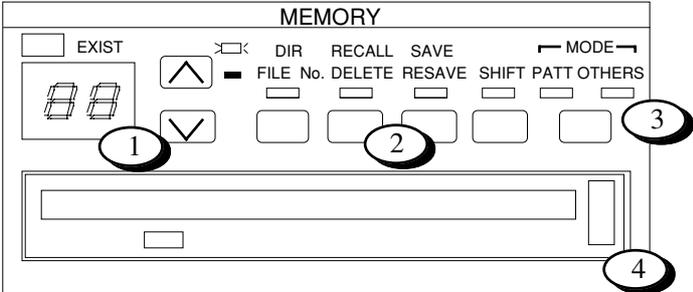

- 1 File No. selection
- 2 File control
- 3 Mode selection
- 4 Eject

SECTION 4 OPERATION

4.6.1 File save

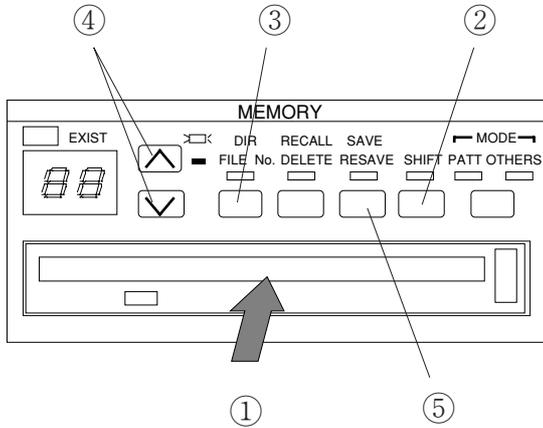


- ① Insert a formatted disk (2HD, 2DD) into the floppy disk drive. (For a description of the formatting method, see Paragraph 4.6.3 Disk formatting.)
- ② Select the PATT mode or OTHERS mode.
PATT mode : Stores the contents set at Paragraph 4.4.
OTHERS mode : Stores the contents other than PATT.
- ③ Press the DIR/File No. key. The File No. LED lights.
- ④ Set the file name (00 to 99) with the keys.
- ⑤ Press the SAVE key and save the file.

* If another file was previously saved under the same file name, the current file cannot be saved with the SAVE key. If the old file is unnecessary, a new file can be saved by pressing the SHIFT key, then pressing the SAVE key. If the old file is necessary, save the new file by changing its file name.

Note: When there is not enough vacant space on the FD to resave files, files cannot be resaved. In this case, to try to resave files, "DELETE" files from the FD.


Files larger than 720 k cannot be resaved to an FD formatted at 1.44 M.

4.6.2 File recall

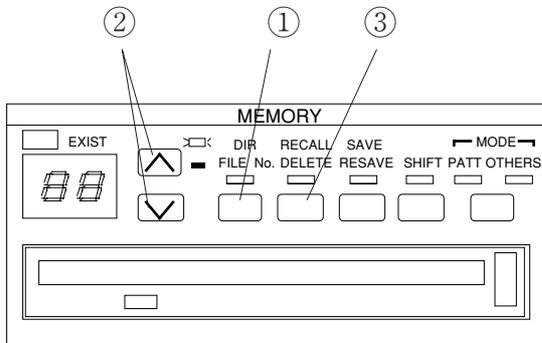

- ① Insert the disk into the floppy disk drive and select the DIR mode. When the FD was changed, always execute the DIR command.
- ② Press the keys and check if the file exists. If the file exists, only its file name is displayed. However, if the file is not on the inserted floppy, "--" is displayed.
- ③ Press the RECALL key and call the contents of the file.

4.6.3 Disk formatting

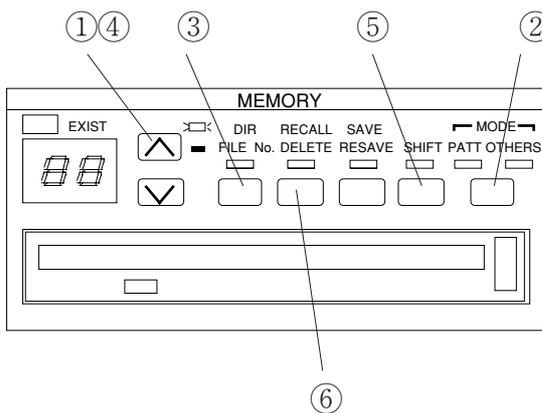


- ① Insert an unformatted floppy disk into the floppy disk drive.
- ② Select the PATT mode or OTHERS mode.
- ③ Select the FILE No. mode.
- ④ Hold down the key. "Fr" is displayed. (Fr is displayed after 99.)
- ⑤ Select the SHIFT mode.
- ⑥ When the DELETE key is pressed, formatting starts.

Note: The formatting format can be switched between 1440 KB/720 KB or 1232 KB/640 KB by rear panel FUNCTION switch. However, if the format was changed, turn the power off, then turn it back on.

SECTION 4 OPERATION

4.6.4 File delete

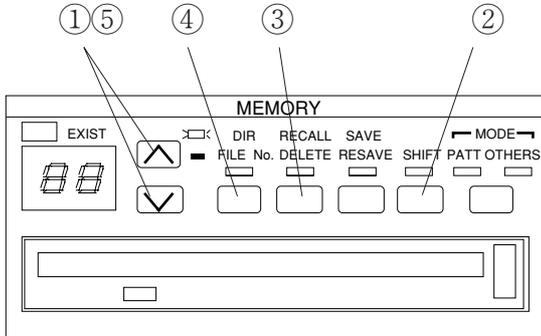

- ① Insert the floppy disk into the floppy disk drive and select the name of the file you want to delete.
- ② Press the SHIFT key.
- ③ Press the DELETE key. The file with the displayed file name is deleted.
- ④ (Confirmation)
Execute the DIR command.
- ⑤ Press the keys and check that the deleted file name is not displayed.

4.6.5 Error messages

When a floppy disk error was generated, an error code of from E0 to E9 is displayed on the file name display. For the error display, see Table 4-5 Error Messages. The error messages are cleared each time the keys are pressed.

Table 4-5 Error Messages

Error item	Error contents
E0	Media error (Formatting, media error)
E1	Write protection error (Protection error when writing)
E2	File full (Write area too small)
E3	File not found (Specified file could not be found when reading.)
E4	File exists error (An attempt was made to save the same file)
E5	Write error (Write obstruction error)
E6	Read error (Read obstruction error)
E7	File type, File error (File type or file contents error)
E8	FD error (Other error)
E9	Hardware error (Hardware trouble error)

4.6.6 Floppy disk

(a) Disk type

Floppy disks are formatted in the standard MS-DOS format provided by the MS-DOS handler. The type of formatted floppy disk is data disk. This is because the MS-DOS file handler does not copy the MS-DOS system. A system disk containing the MS-DOS system can also be used to store data.

(b) Volume label

A volume label is added when the floppy disk is formatted.

Volume label: MP1764A

This volume label is provided to identify the floppy disk.

(c) File structure

- Directory structure

Route directory only.

- File name, extension

The file name and extension have the following format:

File name	<u>RR</u> × ×
	00 to 99 (file name)
Extension	PTN: Pattern file
	OTH: Parameter file other than pattern

Examples: RR99. PTN

RR01. OTH

(d) Data format

The format of the data stored on floppy disk is, as a rule, not made public. Therefore, when data creation, updating, etc. are performed using a personal computer that runs under MS-DOS, operation is not guaranteed. However, there is no problem in checking the file directory or copying files.

(e) Compatibility

The MP1764A Error Detector 'PTN' file mode can be used with the MP1763B Pulse Pattern Generator. The 'OTH' file cannot be used with the MP1763B Pulse Pattern Generator.

The MP1764A cannot read the files of the old MP1702A, MP1609A, and MP1651A Error Detectors.

4.6.7 Floppy disk precautions

- Do not remove a floppy disk from the floppy disk drive while it is being accessed.
- Observe the specified environmental conditions, and do not use the floppy disk in dusty places.
- Clean head of floppy disk drive with 3.5 inch head cleaning disk set regularly.
- Do not place a magnetized object near the floppy disk and do not bend the floppy disk.

SECTION 4 OPERATION


4.7 Printer output

The MP1764A has an GPIB connector for local printer. It is easy to print measurement data.


Five kinds of data are printed: measurement start data, measurement end data, intermediate measurement data, 1 second data, and alarm data.

Not only the measured results, but also threshold EI/EFI and performance data can be printed at the measurement end data and intermediate measurement data.

Printout procedure

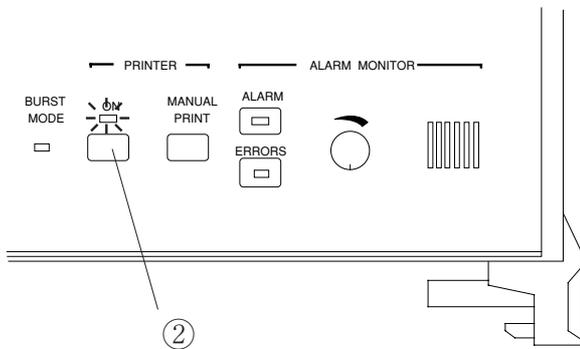

- ① Select the desired print data from Table 4-6 and set the FUNCTION2 switch.
- ② Set the PRINTER key to ON. When the key is ON, the LED lights.

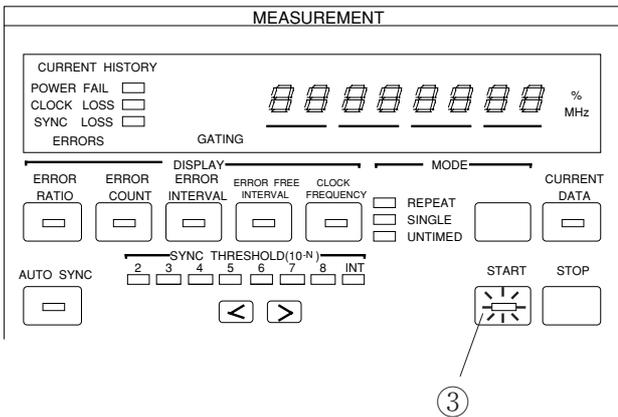

- ③ Press the START key.
- * To print intermediate measurement data, press the MANUAL PRINTER key each time.

The print data contents are shown below.

Table 4-6 Print Data Contents

	Print data contents	Print timing	Printing restriction
Measurement start data	<ul style="list-style-type: none"> Measurement start time 	<ul style="list-style-type: none"> At the start of measurement. 	None
Measurement end data	<ul style="list-style-type: none"> Measurement start time Measurement end time Measurement elapsed time Measured result <ul style="list-style-type: none"> Measurement value <ul style="list-style-type: none"> Error ratio Error count EI count EFI ratio Alarm intervals <ul style="list-style-type: none"> Power failure Clock loss Sync loss Threshold EI and EFI data Error performance data 	<ul style="list-style-type: none"> At the end of measurement 	<ul style="list-style-type: none"> The following can be selected with FUNCTION2 SW1, SW2, and SW3. SW1 <ul style="list-style-type: none"> 0 : Print all measured result 1 : Print only error ratio and error count of measured result SW2 <ul style="list-style-type: none"> 0 : Do not print threshold EI and EFI data. 1 : Print threshold EI and EFI data. SW3 <ul style="list-style-type: none"> 0 : Do not print error performance data. 1 : Print error performance data.
Intermediate measurement data	<ul style="list-style-type: none"> Same as measurement end data. However, the measurement end time is replaced by the intermediate measurement time. 	<ul style="list-style-type: none"> When MANUAL PRINT key pressed. When intermediate data printing is selected: <ol style="list-style-type: none"> When measurement time is less than 2 days, every 2 hours. when measurement time is 2 days or more, every day. In UNTIMED mode, every day. 	<ul style="list-style-type: none"> The following can be selected with FUNCTION2 SW4. <ul style="list-style-type: none"> 0 : Do not print intermediate data. 1 : Print intermediate data. Except for the above, the same as measurement end data.

SECTION 4 OPERATION

Table 4-6 Print Data Contents (Continued)

	Print data contents	Print timing	Printing restrictions															
1 second data	<ul style="list-style-type: none"> • Generation time • 1 second average error ratio • 1 second error count 	<ul style="list-style-type: none"> • Every second 	<ul style="list-style-type: none"> • The following can be selected with FUNCTION2 SW5, SW6, and SW7: <p>SW5 0 : Do not print 1 second data. 1 : Print 1 second data.</p> <p>SW6 and SW7</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 15%;">SW6</th> <th style="width: 15%;">SW7</th> <th style="width: 70%;">Function</th> </tr> </thead> <tbody> <tr> <td style="text-align: center;">0</td> <td style="text-align: center;">0</td> <td>When error > 0, print 1 second data.</td> </tr> <tr> <td style="text-align: center;">0</td> <td style="text-align: center;">1</td> <td>When error > 10^{-6}, print 1 second data.</td> </tr> <tr> <td style="text-align: center;">1</td> <td style="text-align: center;">0</td> <td>When error > 10^{-4}, print 1 second data.</td> </tr> <tr> <td style="text-align: center;">1</td> <td style="text-align: center;">1</td> <td>When error > 10^{-3}, print 1 second data.</td> </tr> </tbody> </table> <p>SW8 0 : Paper save function off 1 : Paper save function on</p>	SW6	SW7	Function	0	0	When error > 0, print 1 second data.	0	1	When error > 10^{-6} , print 1 second data.	1	0	When error > 10^{-4} , print 1 second data.	1	1	When error > 10^{-3} , print 1 second data.
SW6	SW7	Function																
0	0	When error > 0, print 1 second data.																
0	1	When error > 10^{-6} , print 1 second data.																
1	0	When error > 10^{-4} , print 1 second data.																
1	1	When error > 10^{-3} , print 1 second data.																
Alarm data	<ul style="list-style-type: none"> • Power failure generation time • Power failure recovery time • Clock loss generation time • Clock loss recovery time • Sync loss generation time • Sync loss recovery time • Unavailable seconds 	<ul style="list-style-type: none"> • Time alarm generated and when alarm recovered. However, the power failure generation time is when the power is recovered. 	None															

4.7.1 Printing Format

Note: ——— Print data (Differs with the setting state and measurement state)

(1) Measurement start data

<<START	<u>94-03-01 21: 20: 05</u>	<u>REPEAT</u>	<u>99-01: 59: 59 >></u>
	Measurement start time	Measurement mode	Measurement time
	Year-day-time Hour:minute:second	REPEAT	Day-hour:minute:second
		SINGLE	(Not printed for UNTIMED.)
		UNTIMED	

(2) 1 second data

		1 second data generation time Year-day-time Hour: minute: second	
-----		1SEC DATA	-----
TIME	<u>94-03-01 21:20:06</u>		
ERROR RATIO	<u>1.0000E-11</u>	ERROR COUNT	<u>15</u>
-----			-----
	1 second average error ratio measurement		Number of errors in 1 second

(3) Alarm data

- Power failure/power recovery

		Power failure generation time Year-day-time Hour: minute: second
<< POWER FAILURE	<u>94-03-01 21:20:07</u>	>>
<< POWER RECOVERY	<u>94-03-01 21:20:08</u>	>>
		Power recovery time Year-day-time Hour: minute: second

- Clock loss/clock recovery

		Clock loss generation time Year-day-time Hour: minute: second
<< CLOCK LOSS	<u>94-03-01 21:20:09</u>	>>
<< CLOCK RECOVERY	<u>94-03-01 21:20:10</u>	>>
		Clock recovery time Year-day-time Hour: minute: second

SECTION 4 OPERATION

- Sync loss/sync recovery

```

                                Sync loss generation time
                                Year-day-time Hour: minute: second
                                ↓
<< PATTERN SYNC LOSS          94-03-01 21: 20:11          >>

<< PATTERN SYNC RECOVERY      94-03-01 21: 20:12          >>
                                ↑
                                Sync recovery time
                                Year-day-time Hour: minute: second
    
```

(4) Measurement end data and intermediate measurement data

There are two output formats, standard format and abbreviated format. These formats are described below in the order: (a) Standard format and (b) abbreviated format.

(a) Standard format

```

Line 1 *****

Line 2  START    94-03-01 21: 20:13          END          94-03-01 21: 20:14
           ↑           ↑           ↑
           Measurement start time Measurement end data Measurement end time or
           Year-day-time          INT for intermediate intermediate measurement
           Hour: minute: second measurement data          time

Line 3  ----- ERROR MEASUREMENT -----

Line 4  ERROR RATIO    1.0000E-11          ERROR COUNT    25
           ↑           ↑
           Average error ratio          Number of errors

Line 5  ERROR INTVL    1          %ERROR FREE INTVL    0
           ↑           ↑
           Number of error intervals          Error free intervals ratio

Line 6  POWER FAIL INTVL    0          CLOCK LOSS INTVL    0
           ↑           ↑
           Number of power fail intervals          Number of clock loss intervals

Line 7  SYNC LOSS INTVL    0
           ↑
           Number of sync loss intervals

Line 8  -----

Line 9  *****
    
```

4.7 Printer output

When there is threshold EI/EFI data to be printed, the following data is printed between lines 8 and 9.

Line 9 - - - - - THRESHOLD EI. EFI - - - - -

Line 10	ERROR RATIO	ERROR INTVL	%ERROR FREE INTVL
---------	-------------	-------------	-------------------

Line 11	>1.0E-3	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 12	>1.0E-4	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 13	>1.0E-5	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 14	>1.0E-6	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 15	>1.0E-7	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 16	>1.0E-8	$\frac{0}{\quad}$	$\frac{100.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 17	=<1.0E-8	$\frac{1}{\quad}$	$\frac{0.0000\%}{\quad}$
		↙ Number of threshold EI	↙ Threshold EFI ratio

Line 18 - - - - -

SECTION 4 OPERATION

When there is error performance data to be printed, the following data is printed after line 19 (between lines 8 and 9 when threshold EI/EFI data is not printed).

Line 19 ----- ERROR PERFORMANCE -----
(Line 9)

Line 20	%ERRORED SECOND	<u>100.0000%</u>	%ERROR FREE SECOND	<u>0.0000%</u>
(Line 10)		↙		↙
		Error seconds ratio		Error free seconds ratio

Line 21	%SES (1.0E-3)	<u>0.0000%</u>	%DM (1.0E-3)	<u>0.0000%</u>
(Line 11)		↙		↙
		Severely errored seconds ratio		Degraded minutes ratio

Line 22	%UNAVAIL SECOND	<u>0.0000%</u>		
(Line 12)		↙		
		Unavailable seconds ratio		

Line 23 -----
(Line 13)

(b) Abbreviated format

Line 1 *****

Line 2	START	<u>94-03-01 21: 20:13</u>	END	<u>94-03-01 21: 20:14</u>
		↙	↙	↙
		Measurement start time	Measurement end data	Measurement end time or
		Year-day-time	INT for intermediate	intermediate measurement
		Hour:minute:second	measurement data	time

Line 3 ----- ERROR MEASUREMENT -----

Line 4	ERROR RATIO	<u>1.0000E-11</u>	ERROR COUNT	<u>25</u>
		↙		↙
		Average error ratio		Number of errors

Line 5 -----

Line 6 *****

Note: The threshold EI/EFI data and error performance data printing format is the same as the standard output format. The data is printed from line 4.

4.8 Definition of Terms

4.8.1 Measurement items

- (1) Error ratio

$$\frac{\text{Number of error pulses in measurement time}}{\text{Number of clock pulses in measurement time}}$$

- (2) Error count

Number of error pulses in measurement time.

- (3) Error intervals (EI) count

Number of intervals (1 second) containing one or more error pulses in measurement time.

- (4) Error free intervals (EFI) ratio

Ratio of total number of intervals with number of intervals (1 second) containing one or more error pulses to total number of intervals in measurement time. It is calculated from EI with the following equation:

$$\text{EFI} = \left(\frac{\text{number of measurement intervals} - \text{EI}}{\text{Number of measurement intervals}} \right) \times 100\%$$

- (5) Clock frequency

One second clock frequency.

4.8.2 Alarm intervals

- (1) Power failure alarm intervals

Number of intervals (1 second) at which a power failure occurred.

- (2) Clock loss intervals

Number of intervals (1 second) at which a clock loss alarm was generated.

- (3) Sync loss intervals

Number of intervals (1 second) at which a sync loss alarm was generated.

4.8.3 Threshold EI and EFI data

- (1) Threshold EI

Number of intervals (1 second) that the 1 second average error ratio satisfies each of the following thresholds in the measurement time.

$$1 \text{ second average error ratio} > 10^{-3}, > 10^{-4}, > 10^{-5}, > 10^{-6}, > 10^{-7}, > 10^{-8}, \leq 10^{-8}$$

- (2) Threshold EFI

Ratio of the number of intervals at which the 1 second average error ratio does not satisfy each threshold condition of item (1) to the total number of intervals.

The threshold EFI is calculated from EI with the following equation:

$$\text{Threshold EFI} = \left(\frac{\text{Number of measurement intervals} - \text{threshold EI}}{\text{Number of measurement intervals}} \right) \times 100\%$$

SECTION 4 OPERATION

4.8.4 Error performance data

The interval from the start of measurement to the end of measurements is divided into available periods and unavailable periods, with 1 second interval as the unit. Each item is calculated for the available periods.

(1) Definition of unavailable period and available period

When an interval at which the 1 second average error ratio exceeds the unavailable threshold (unavailable period) continues for 10 seconds, the unavailable period starts and this 10 seconds is included in the unavailable seconds.

When an interval at which the 1 second average error ratio does not exceed the unavailable threshold (available interval) continues for 10 seconds in an unavailable period, the unavailable period ends and this 10 seconds is included in the available seconds.

Each is subdivided into two states, with the periods that are not unavailable periods as available periods.

- Unavailable period (after confirmation)

This is the state after the last interval was calculated in the unavailable seconds. When an interval is an unavailable interval, it is calculated in the unavailable seconds and the state does not change.

When an interval is an available interval, the unavailable seconds and available seconds do not change and the state changes to unavailable seconds (during judgment).

- Unavailable period (during judgment)

This is the state during which whether the last interval was included in unavailable seconds or available seconds during an unavailable interval is judged.

When the interval is an unavailable interval, the continuation seconds of this state is calculated in the unavailable seconds and the state changes to unavailable period (after confirmation).

When the interval is an available interval, and the number of consecutive available intervals reached 10, the continuation time of this state (=10 seconds) is calculated in the available seconds and the state changes to available period (after confirmation). When the number of consecutive available intervals is less than 10, the unavailable seconds and available seconds do not change and this state continues.

- Available period (after confirmation)

This is the state after the last interval was calculated in the available seconds.

When the interval is an available interval, it is calculated in the available seconds and the state does not change.

When the interval is an unavailable interval, the available seconds and unavailable seconds do not change and the state changes to available seconds (during judgment).

4.8 Definition of Terms

- Available seconds (during judgment)

This is the state during which whether the last interval is included in the available seconds in an available period.

When the interval is an available interval, the continuation time of that state is calculated in the available seconds and the state changes to available period (after confirmation).

When the interval is an unavailable interval, and the number of consecutive unavailable intervals reached 10, the continuation time (=10 seconds) of this state is calculated in the unavailable seconds and the state changes to unavailable period (after confirmation). When the number of consecutive unavailable intervals is less than 10, the available seconds and unavailable seconds do not change and this state is continued.

The initial state is available period (after confirmation).

- (2) Unavailable threshold, DM threshold

The following can be selected with FUNCTION1 SW4:

0: Unavailable threshold = 10^{-3} , DM threshold = 10^{-6}

1: Unavailable threshold = 10^{-4} , DM threshold = 10^{-8}

- (3) Measurement items

- Unavailable Seconds

Ratio of unavailable seconds to measurement time.

- Error Seconds

Ratio of error intervals calculated in available seconds to all intervals calculated in available seconds.

- Error Free Seconds

Ratio of error free intervals calculated in available seconds to all intervals calculated in available seconds.

- Severely Errored Seconds (SES)

Ratio of unavailable intervals calculated in available seconds to all intervals calculated in available seconds.

- Degraded Minutes

The error ratio is calculated for every 60 packets, excluding the SES above at the available interval calculated in the available seconds. The error ratio is the ratio of the number of packets exceeding the DM threshold to the total number of packets.

SECTION 4 OPERATION

4.9 Processing of Measurement Data At Alarm Generation

(1) Power failure

When a power failure alarm is generated during measurement, the measurement data up to the interval before the interval that generated the power failure alarm is saved during the power failure.

If the measurement data was correctly saved, measurement is continued after the power recovers.

(a) Error measurement

The number of error pulses and the number of clock pulses counted in the interval that generated the power failure alarm are removed from calculation.

(b) Interval measurement, threshold interval measurement

The interval that generated the power failure alarm and the interval during continuation of the power failure are included only in the power failure intervals calculation and are included in other calculations.

(c) Error performance

The interval being judged when a power failure alarm was generated is not included in neither unavailable seconds nor available seconds calculation.

After the power recovers, measurement restarts from the initial state.

(2) Clock loss

When a clock loss alarm is generated during measurement, one of the following two processings can be selected:

(a) Removal of clock loss processing from calculation (FUNCTION1 SW2 set to 0.)

(i) Error measurement

The number of error pulses and number of clock pulses counted in the interval that generated the clock loss alarm are removed from calculation.

(ii) Interval measurement, threshold interval measurement

Intervals whose interval status is clock loss are included in clock loss intervals calculation only. They are not included in other calculations.

(iii) Error performance

Intervals whose interval status is clock loss are not included in neither unavailable seconds or available seconds calculation. The interval being judged is not included in unavailable seconds or available seconds calculation either.

When the interval status is no longer clock off, measurement is continued from the initial state.

4.9 Processing of Measurement Data At Alarm Generation

(b) Inclusion of clock loss processing in calculation (FUNCTION1 SW2 set to 1.)

(i) Error measurement

The number of error pulses and number of clock pulses counted in the interval that generated the clock loss alarm are removed from calculation.

(ii) Interval measurement, threshold interval measurement

Intervals whose interval status is clock loss are included in clock loss intervals and total intervals calculation, but are not included in threshold EI calculation.

(iii) Error performance

Intervals whose interval status is clock loss become unavailable intervals and when they were included in available seconds calculation, they are also included in error seconds calculation.

(3) Sync loss

When a sync loss alarm is generated during measurement, one of the following two processings can be selected:

(a) Removal of sync loss processing from calculation (FUNCTION1 SW3 set to 0)

(i) Error measurement

The number of error pulses and number of clock pulses counted in the interval that generated the sync loss alarm are removed from calculation.

(ii) Interval measurement, threshold interval measurement

Intervals whose interval status is sync loss are included only in sync loss intervals calculation. They are not included in other calculations.

(iii) Error performance

Intervals whose interval status is sync loss are not included in neither unavailable seconds nor available seconds calculation. The interval being judged is not included in unavailable seconds and available seconds calculations either.

When the interval status is not longer sync loss, measurement is continued from the initial state.

(b) Inclusion of sync loss processing in calculations (FUNCTION1 SW3 set to 1.)

(i) Error measurement

The number of error pulses and the number of clock pulses counted in the interval that generated the sync loss alarm are removed from all calculations.

(ii) Interval measurement, threshold interval measurement

Intervals whose interval status is sync loss are included in sync loss intervals and total intervals calculations, but are not included in threshold EI calculation.

(iii) Error performance

Intervals whose interval status is sync loss become unavailable intervals and when they were included in available seconds calculation, they are also included in error seconds calculation.

SECTION 4 OPERATION

4.10 FUNCTION Switch Setting

The setting contents of the FUNCTION1 and 2 switches on the rear panel of the mainframe show below.

When the FUNCTION2 SW10 setting was changed, turn on the mainframe power again.

* When the setting of the other FUNCTION switches was changed, the power does not have to be turned on again.

Note: When the system control setting was changed, turn on the power again.

4.10 FUNCTION Switch Setting

FUNCTION 1

	Marking	Function															
1	BIT SHIFT NUMBER FOR MARK RATIO VARIED	Number of AND shift bits at mark ratio setting switch 0 : 1 bit 1 : 3 bits															
2	CLOCK LOSS EVALUATION	Clock loss processing function selector switch 0 : Do not measure and evaluate clock loss 1 : Measure and evaluate clock loss															
3	SYNC LOSS EVALUATION	Sync loss processing function selector switch 0 : Do not measure and evaluate sync loss 1 : Measure and evaluate sync loss															
4	ERROR PERFORMANCE THRESHOLD	Error performance threshold selector switch 0 : 10^{-3} 1 : 10^{-4}															
5	BURST MODE	Burst mode switch 0 : OFF 1 : ON															
6	CURRENT DATA CALCULATION	Calculation mode of intermediate measurement data displayed when CURRENT DATA key ON selector switch 0 : Progressive mode 1 : Immediate mode															
7, 8	ERROR	Error detection mode selector switch <table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>SW7</th> <th>SW8</th> <th>Error mode</th> </tr> </thead> <tbody> <tr> <td>0</td> <td>0</td> <td>Total error</td> </tr> <tr> <td>0</td> <td>1</td> <td>Insertion error</td> </tr> <tr> <td>1</td> <td>0</td> <td>Omission error</td> </tr> <tr> <td>1</td> <td>1</td> <td>Total error</td> </tr> </tbody> </table>	SW7	SW8	Error mode	0	0	Total error	0	1	Insertion error	1	0	Omission error	1	1	Total error
SW7	SW8	Error mode															
0	0	Total error															
0	1	Insertion error															
1	0	Omission error															
1	1	Total error															
9, 10	INTERVAL TIME	INTERVAL TIME selector switch (at the EI or %EFI measurement) <table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>SW9</th> <th>SW10</th> <th>Cycle time</th> </tr> </thead> <tbody> <tr> <td>0</td> <td>0</td> <td>1 ms</td> </tr> <tr> <td>0</td> <td>1</td> <td>10 ms</td> </tr> <tr> <td>1</td> <td>0</td> <td>100 ms</td> </tr> <tr> <td>1</td> <td>1</td> <td>1 s</td> </tr> </tbody> </table>	SW9	SW10	Cycle time	0	0	1 ms	0	1	10 ms	1	0	100 ms	1	1	1 s
SW9	SW10	Cycle time															
0	0	1 ms															
0	1	10 ms															
1	0	100 ms															
1	1	1 s															

SECTION 4 OPERATION

FUNCTION 2

	Marking		Function															
1	SHORT FORM OUTPUT		Measurement data printing format selector switch 0 : Standard format 1 : Abbreviated format															
2	THRESHOLD EI, EFI DATA		Switch that selects whether or not threshold EI and EFI data are printed. 0 : Do not print 1 : Print															
3	ERROR PERFORMANCE DATA		Switch that selects whether or not error performance data is printed. 0 : Do not print 1 : Print															
4	INTERMEDIATE DATA		Switch that selects whether or not intermediate data is printed. 0 : Do not print 1 : Print															
5	ONE SECOND DATA	OUTPUT	Switch that selects whether or not 1 second data is printed. 0 : Do not print 1 : Print															
6,7		OUTPUT THRESHOLD	1 second data printing threshold selector switch <table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>SW6</th> <th>SW7</th> <th>Error threshold</th> </tr> </thead> <tbody> <tr> <td>0</td> <td>0</td> <td>> 0</td> </tr> <tr> <td>0</td> <td>1</td> <td>> 10⁻⁶</td> </tr> <tr> <td>1</td> <td>0</td> <td>> 10⁻⁴</td> </tr> <tr> <td>1</td> <td>1</td> <td>> 10⁻³</td> </tr> </tbody> </table>	SW6	SW7	Error threshold	0	0	> 0	0	1	> 10 ⁻⁶	1	0	> 10 ⁻⁴	1	1	> 10 ⁻³
SW6		SW7	Error threshold															
0	0	> 0																
0	1	> 10 ⁻⁶																
1	0	> 10 ⁻⁴																
1	1	> 10 ⁻³																
8	PAPER SAVING	Switch that selects whether or not printer paper is saved. 0 : Do not save 1 : Save																
9	CURRENT DATA INTERVAL		Switch that selects the current data measurement time. 0 : 100 ms 1 : 200 ms															
10	FD FORMATTING TYPE		Switch that selects the floppy disk format. 0 : 1440 K / 720 KB 1 : 1232 K / 640 KB															

SECTION 5

PRINCIPLE OF OPERATION

5.1 Pseudorandom Pattern (PRBS Pattern)







The principle of pseudorandom pattern generation is shown in Table 5-1. The pseudorandom pattern is represented by the N-order generation polynomial shown in Table 5-1. One period is 2^N-1 . A PRBS pattern with a 2^N-1 period produces an N bits continuous "1" pattern per period.

When LOGIC is set to POS (positive logic), PRBS pattern output level "1" corresponds to low level and "0" corresponds to high level.

The PRBS pattern mark ratio is generated by the block shown in Fig. 5-1. There are four mark ratios of 1/2, 1/4, 1/8, and 0/8 (all 0). For 1/4 and 1/8, 2 bit shift or 3 bit shift can be selected by rear panel DIP switch. (See Paragraph 4.10 FUNCTION Switch Setting.)

When the rear panel 1/8 SPEED output is PRBS pattern, a pattern like that shown in Fig. 5-2 is produced.

Table 5-1 Principle of Pseudorandom Pattern Generation

Period	Generation polynomial	Pattern generation block diagram
2^7-1	$1+X^6+X^7$	
2^9-1	$1+X^5+X^9$	
$2^{11}-1$	$1+X^9+X^{11}$	
$2^{15}-1$	$1+X^{14}+X^{15}$	
$2^{20}-1$	$1+X^3+X^{20}$	
$2^{23}-1$	$1+X^{18}+X^{23}$	
$2^{31}-1$	$1+X^{28}+X^{31}$	

□ : Shift register

⊕ : Exclusive-OR

SECTION 5 PRINCIPLE OF OPERATION

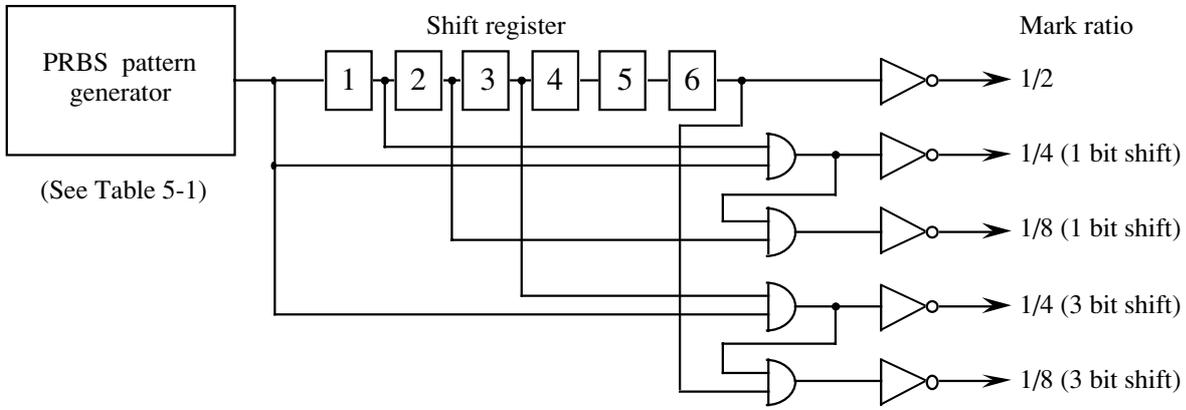


Fig. 5-1 Mark Ratio 1/4, 1/8 Pattern Generation Circuit

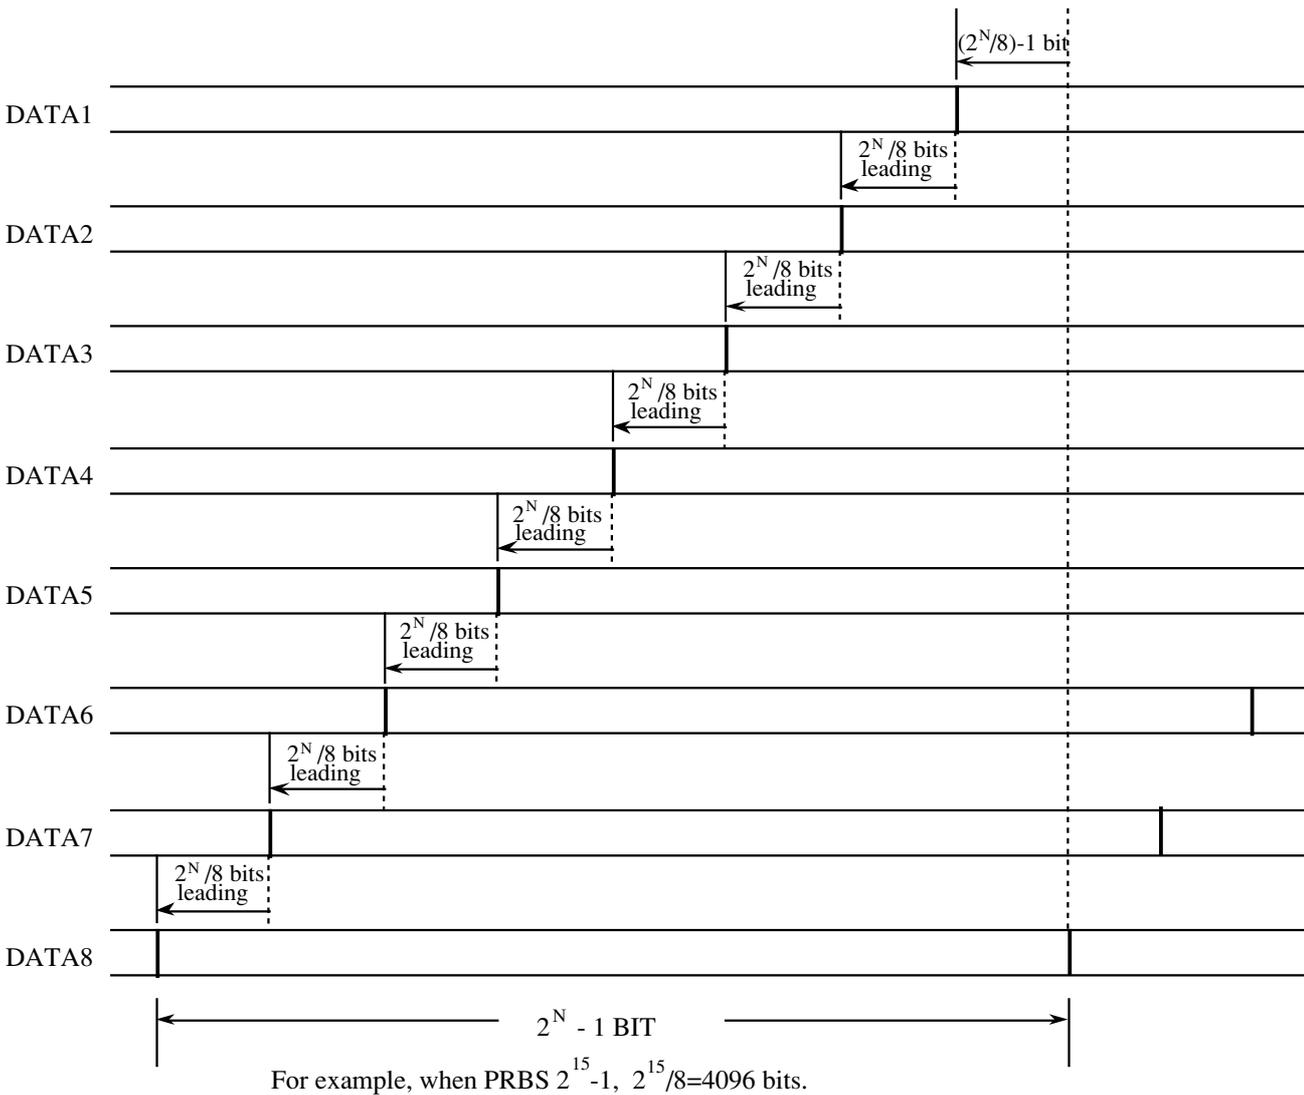


Fig. 5-2 Example of Pseudorandom Pattern

5.2 Pattern Synchronized Output Synchronization

5.2.1 Pseudorandom pattern

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times (2^N - 1) \times 32$$

$$N=7, 9, 11, 15, 20, 23, 31$$

$$\text{(Where pulse width} = \frac{1}{(\text{Set frequency})} \times 32 \text{ plus pulses)}$$

5.2.2 Programmable pattern

(1) Data pattern, alternate pattern

(a) Data length = 65536 or less

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times (128 \text{ and lowest common denominator of data length})$$

(Example 1) Data = 8

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times 128$$

(Example 2) Data = 10

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times 640$$

(b) Data length > 65536

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times (\text{data length})$$

(2) Zero Sub pattern

$$\text{Period} = \frac{1}{(\text{Set frequency})} \times 2^N \quad N=7, 9, 11, 15$$

(3) Pulse width

For any of the programmable patterns above, the pulse width is pulse width = $\frac{1}{(\text{Set frequency})} \times 32$. The output signal polarity is plus pulse.


Note: For alternate pattern, the sync pulse is output in basic data length units. When the data output is observed with a sampling oscilloscope, pattern A and pattern B appear to be superimposed.

When you want to observe the data output pattern A or pattern B without being superimposed, input the rear panel A/B TIMING OUTPUT of MP1763B to a sampling oscilloscope trigger via an ECL terminator.

SECTION 5 PRINCIPLE OF OPERATION

5.3 Frame Sync Output

The frame sync pulse is output when the frame sync function is on. Its period and pulse width are shown in Fig. 5-3.

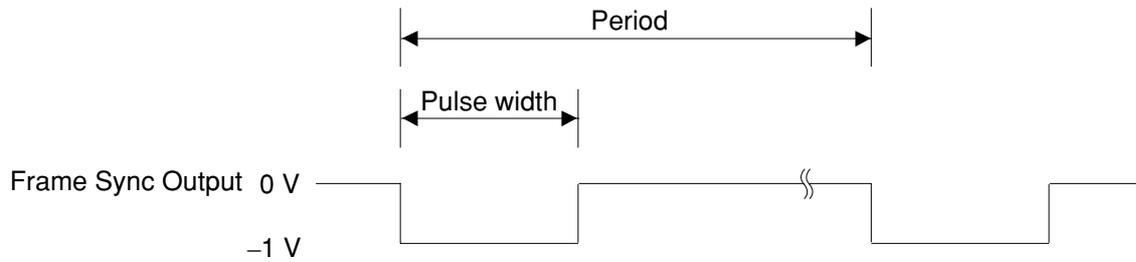

- Pulse width = $\frac{1}{(\text{Set frequency})} \times 32$

- The period is the same as the pattern sync output period. See Paragraph 5.2.
- Not output when the bit length is 128 bits.

Fig. 5-3 Frame Sync Output

5.4 Error Output

The error output can be of two types, direct error and stretched error. The error detection block diagram is shown in Fig. 5-4 and the error output pulse is illustrated in Fig. 5-5.

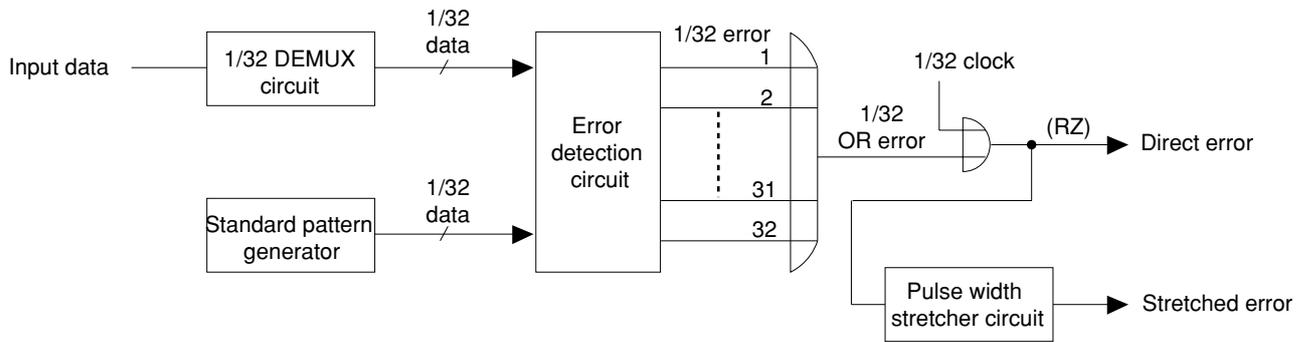


Fig. 5-4 Error Output Block Diagram

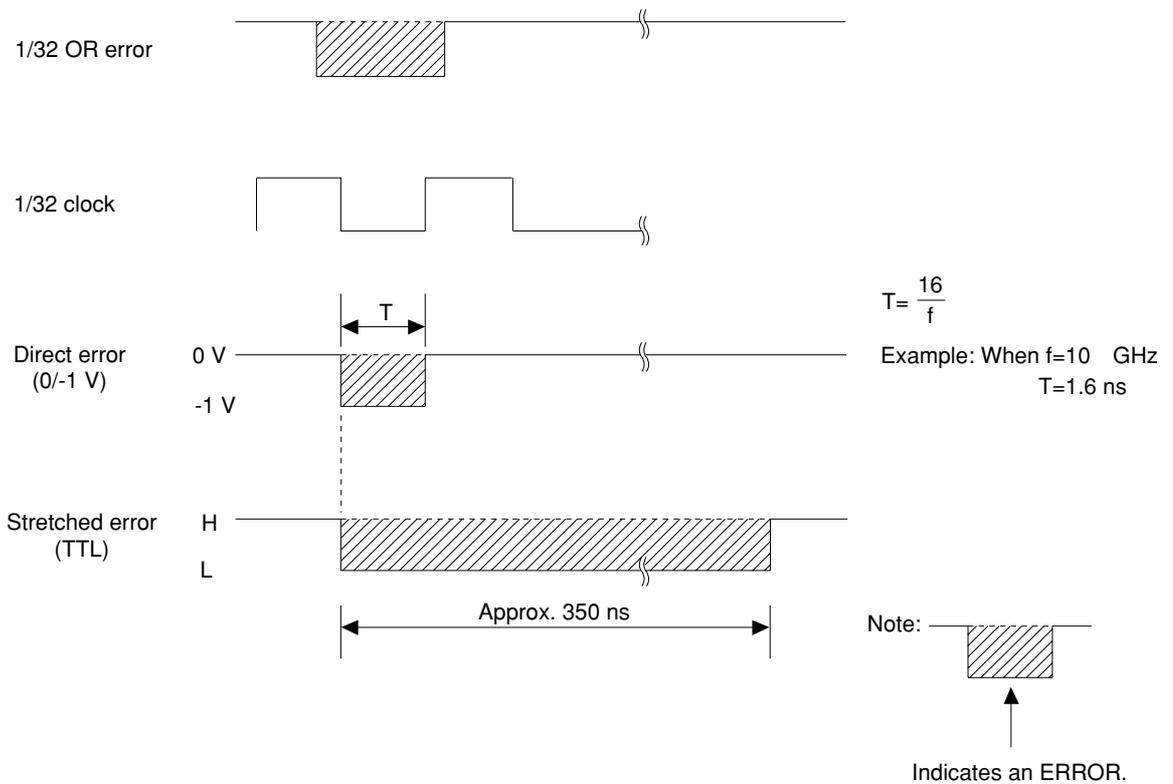


Fig. 5-5 Error Output Pulse


SECTION 5 PRINCIPLE OF OPERATION

(Blank)

SECTION 6 MEASUREMENT

This section describes an example of DFFIC evaluation using the MP1764A Error Detector and MP1763B Pulse Pattern Generator.

6.1 Set-up

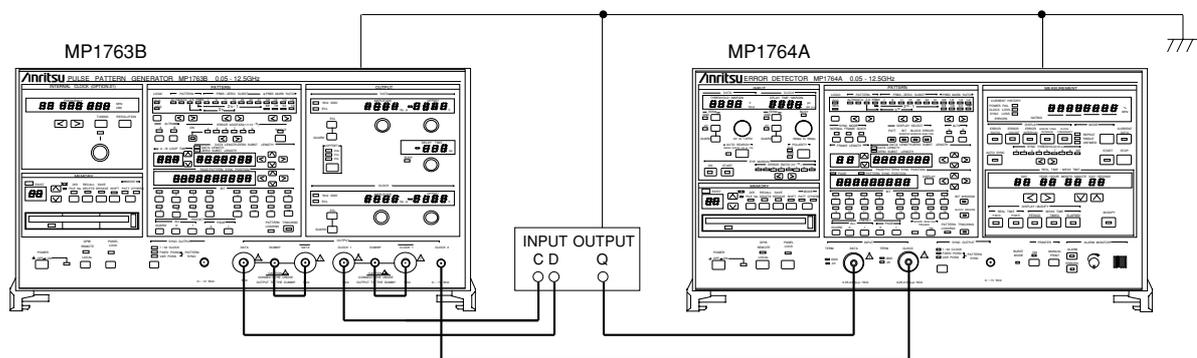

- (1) Ground the system by connecting GND of the measuring instruments and the device under test.
- (2) Connect the power cord.
- (3) Connect the input/output signals using the accessory semirigid cable or an equivalent coaxial cable. At this time, short the center conductor of the cable with tweezers, etc. before use.



6.2 Measurement

- (1) Initialize the MP1763B and MP1764A. Set the POWER switch to ON while pressing the LOCAL key.
- (2) Set the MP1763B DATA and CLOCK1 outputs to ECL level (offset: $0.8V_{OH}$, level: $0.9V_{p-p}$). Set the DUMMY termination to -2 V.
- (3) Set the MP1764A termination condition to -2 V.
- (4) Turn on the power of the device under test.
- (5) Set the MP1763B frequency to the measurement frequency, and the OUTPUT to ON.
- (6) Press the MP1764A AUTO SYNC key, then press the AUTO SEARCH key. After the end of AUTO SEARCH, check that all the error and alarm lamps are off. If an error lamp is lit, change the MP1763B CLOCK phase.
- (7) While watching the MP1764A ERRORS lamp, change the MP1763B offset voltage and amplitude and measure the input level margin of the IC under test.

SECTION 6 MEASUREMENT

6.3 Burst Measurement

To perform the burst measurement, set the function sw5 (BURST MODE) on the MP1764A rear panel to ON and connect the MP1764A to the MP1763B and DUT as shown below:

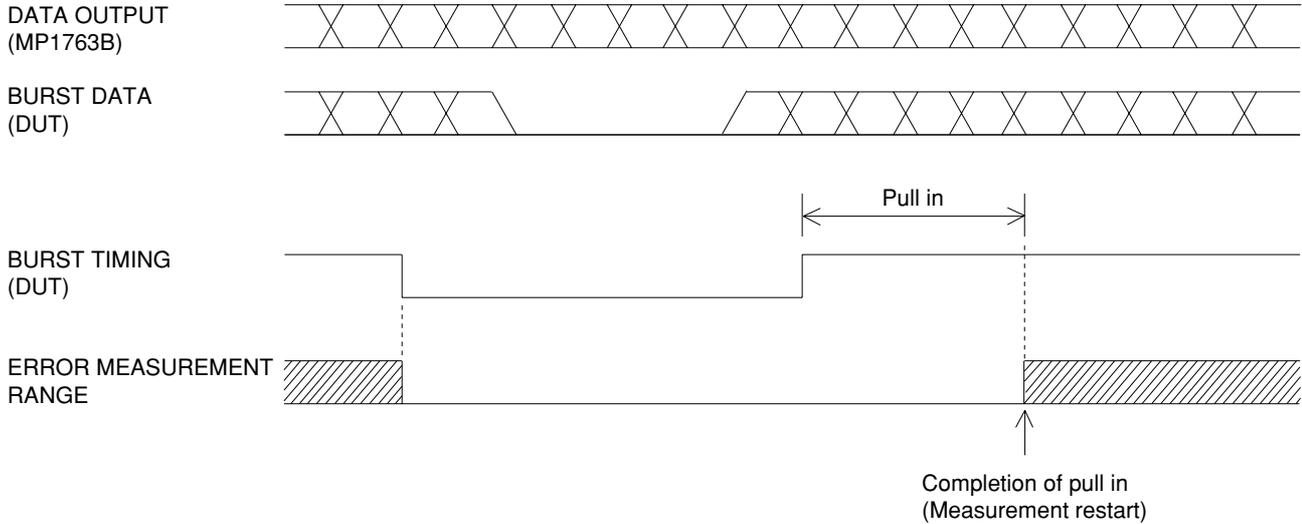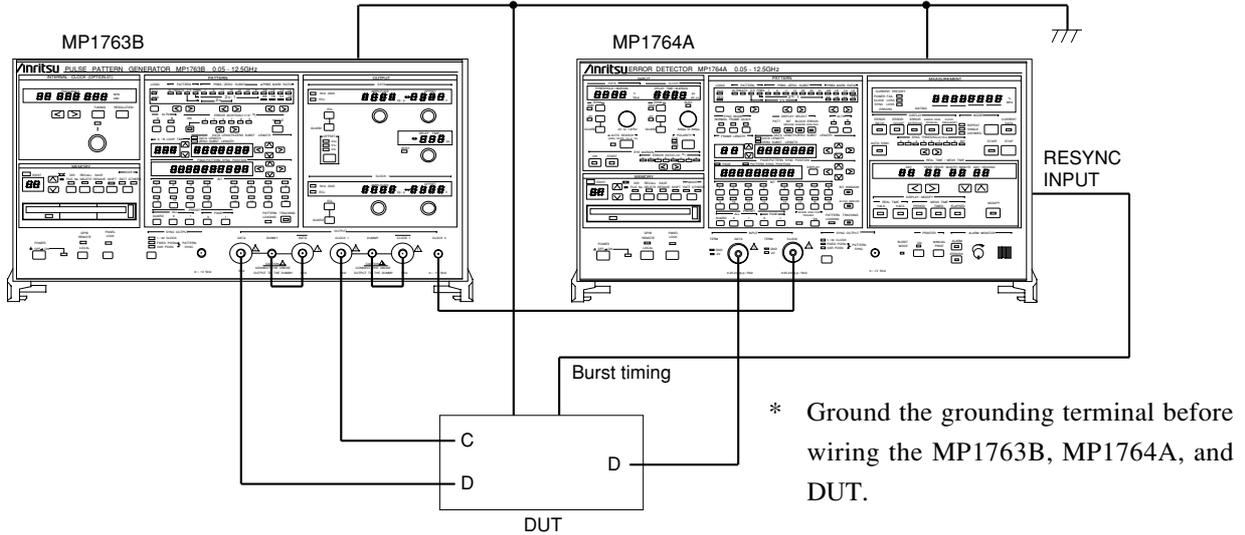

Burst measurement

Restart the burst measurement after termination of the burst timing and completion of pull in. In other words, the measurement inhibiting time is the time of burst timing added by the pull-in time.

SECTION 7 PERFORMANCE CHECK

7.1 When Performance Check Necessary

Performance checks are performed to check that the main performances of the MP1764A satisfy the ratings. Carry out the performance checks during receiving inspection, operation confirmation after repair, and periodic inspection (every six months).

The performance check items are shown below.

7.2 Test Equipment

The test equipment needed for performance check are shown in Table 7-1.

Table 7-1 Performance Check Test Equipment

Test equipment name (Anritsu)	Required performance	Measurement item
Pulse pattern generator (MP1763B)	Operating frequency: 50 MHz to 12.5 GHz Other performances: Equivalent to MP1763B	<ul style="list-style-type: none"> • Operating frequency • Input level • Pattern • Measurement items
Sampling oscilloscope	Bandwidth: 50 GHz minimum	

SECTION 7 PERFORMANCE CHECK

7.3 Check Method

Before starting performance checks, allow the MP1764A and the other test equipment to warm up for at least 30 minutes.

7.3.1 Operating frequency

(1) Rating

50 MHz to 12.5 GHz

(2) Setup

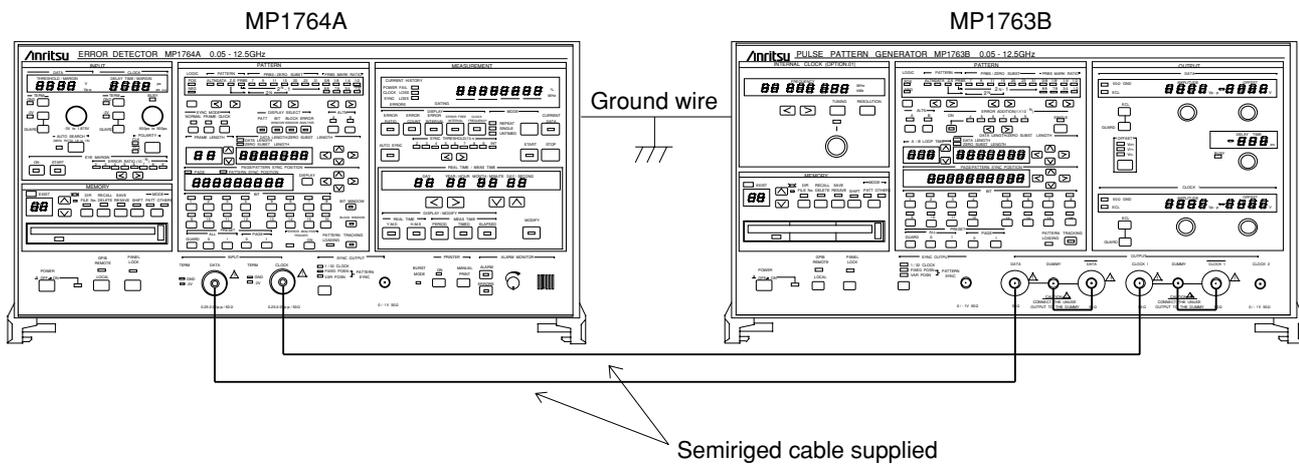


Fig. 7-1 MP1763B and MP1764A Setup

(3) Procedure

(a) Set up the equipment as shown in Fig. 7-1.

(b) While pressing the MP1763B and MP1764A LOCAL key, set the POWER switch to ON and place the instruments into the initialize state. Then, set the MP1763B OUTPUT to ON, and press the MP1764A AUTO SYNC key.

(c) Set the MP1763B FREQUENCY to an arbitrary value with the frequency setting knob.

(d) Press the MP1764A AUTO SEARCH key. At this time, check that the ERRORS lamp at the MP1764A display is not lit.

(e) Repeat steps (c), (d) and confirm that the MP1764A operates normally.

7.3.2 Input data level

(1) Rating

Amplitude : 0.25 to 2 V_{p-p}

Offset (V_{OH}) : -2 to +2 V

Threshold voltage : -3 to +1.875 V

(2) Setup

The setup method is the same as Paragraph 7.3.1(2) and is shown in Fig. 7-1.

(3) Procedure

(a) Set up the equipment as shown in Fig. 7-1.

(b) While pressing the MP1763B and MP1764A LOCAL key, set the POWER switch to ON and set the instruments to the initialize state. Then, set the MP1763B OUTPUT and the MP1764A AUTO SYNC to ON.

(c) When the following was effected, check that the ERRORS lamp is not lit. However, set the input clock and input data phase suitably with the DELAY TIME value setting knob.

Note: Since the MP1764A THRESHOLD value shown below is the logic value, measure the MP1763B data output level in advance with a calibrated sampling oscilloscope, then set the MP1764A THRESHOLD value to the correct value.

Setting order	MP1763B		MP1764A	
	DATA		DATA	
	AMPLITUDE	OFFSET (V _{OH})	TERM	THRESHOLD
①	2.000 V _{p-p}	-2.000 V	GND	-3.000 V
②	0.250 V _{p-p}	-2.000 V	GND	-2.125 V
③	2.000 V _{p-p}	2.000 V	GND	1.000 V
④	0.250 V _{p-p}	2.000 V	GND	1.875 V
⑤	0.800 V _{p-p}	-0.900 V	-2 V	-1.300 V

SECTION 7 PERFORMANCE CHECK

7.3.3 Input clock level

(1) Rating

Amplitude : 0.25 to 2 Vp-p

Offset (V_{OH}) : -2 to +2 V

(2) Setup

The setup method is the same as Paragraph 7.3.1(2) and is shown in Fig. 7-1.

(3) Procedure

(a) Set up the equipment as shown in Fig. 7-1.

(b) While pressing the MP1763B and MP1764A LOCAL key, set the POWER switch to ON and set the instruments to the initialize state. Then, set the MP1763B OUTPUT and the MP1764A AUTO SYNC to ON.

(c) When the following was effected, confirm that the ERRORS lamp did not light. However set the input clock and input data phases suitably with the DELAY TIME setting knob.

Note: Since the MP1764A THRESHOLD value below is the logic value, measure the MP1763B data output level in advance with a calibrated sampling oscilloscope, then set the MP1764A THRESHOLD value to the correct value.

Setting order \ Item	MP1763B		MP1764A
	CLOCK 1		CLOCK TERM
	AMPLITUDE	OFFSET (V _{OH})	
①	2.000 Vp-p	-2.000 V	GND
②	0.250 Vp-p	-2.000 V	GND
③	2.000 Vp-p	2.000 V	GND
④	0.250 Vp-p	2.000 V	GND
⑤	0.800 Vp-p	-0.900 V	-2 V

7.3.4 Pattern

(1) Rating

Pseudorandom (PRBS) pattern

Programmable (PRGM) pattern

Data mode Data length: 2 to 8388608 bits

(2) Setup

The setup method is the same as Paragraph 7.3.1(2) and is shown in Fig. 7-1.

(3) Procedure

(a) Set up the equipment as shown in Fig. 7-1.

(b) While pressing the MP1763B and MP1764A LOCAL key, set the POWER switch to ON and set the instruments to the initialize state. Then, set the MP1763B OUTPUT and the MP1764A AUTO SYNC to ON.

(c) Press the MP1764A AUTO SEARCH key.

(d) Set the MP1763B and MP1764A pattern mode to programmable data pattern and make the settings shown below. At this time, confirm that the ERRORS lamp does not light.

Setting order	Item	Setting
①	DATA LENGTH value	8
②	BIT key	1
		2 to 8
		ON (LED lit)
		OFF (LED off)

(e) Change the MP1763B and MP1764A pattern mode to PRBS 2^7-1 , PRBS 2^9-1 , PRBS $2^{11}-1$, PRBS $2^{15}-1$, PRBS $2^{20}-1$, PRBS $2^{23}-1$, and PRBS $2^{31}-1$ and check that the ERRORS lamp does not light at each mode.

(f) Fix the MP1763B and MP1764A pattern mode at PRBS $2^{31}-1$ and change the mark ratio $0/8$, $1/8$, $1/4$, $1/2$, $8/8$, $7/8$, $3/2$, and $1/2$ and check that the ERRORS lamp does not light at each mark ratio.

SECTION 7 PERFORMANCE CHECK

7.3.5 Measurement items

(1) Rating

Error rate	: $0.0000 \times 10^{-16} = 1.0000 \times 10^{-5}$
Error count	: 0 to 9.9999×10^{16}
Error intervals I(EI)	: 0 to 9999999
Error free intervals (EFI)	: 0.0000 to 100.0000%
Clock frequency	: 50 MHz to 12.5 GHz
	Accuracy: $\pm(10 \text{ ppm} + 1 \text{ kHz})$

(2) Setup

The setup method is the same as Paragraph 7.3.1(2) and is shown in Fig. 7-1.

(3) Procedure

(a) Set up the equipment as shown in Fig. 7-1.

(b) While pressing the MP1763B and MP1764A LOCAL key, set the POWER switch to ON and set the instruments to the initialize state. Set the MP1763B OUTPUT to ON, and the frequency to 10 GHz.

(c) Set the MP1764A AUTO SYNC to ON, and press the AUTO SEARCH key.

(d) Turn on the MP1763B error addition function. (Error addition: Single)

(e) Set the MP1764A measurement mode to SINGLE and set the measurement time to 10 seconds.

(f) Press the MP1764A START key. After the GATING lamp lights, press the MP1763B ERROR ADDITION SINGLE key once.

After the end of measurement (after 10 seconds), switch the DISPLAY key and check if each value shown below is displayed.

Error ratio	: 1.0000E-11
Error count	: 1
Error intervals	: 1
Error free intervals	: 99.9900%
Clock frequency	: 9999.899 to 10000.101 MHz

SECTION 8 MAINTENANCE

8.1 Daily Maintenance

The daily maintenance method and maintenance period are shown in Table 8-1.

Table 8-1

Item	Period	Maintenance method
Exterior soiling	· Before long-term storage	Wipe with a cloth dipped in dilute neutral cleanser.
Dust	· When used in a dusty place	Blow off with compressed air. Clean head of floppy disk drive with 3.5 inch head cleaning disk set.
Loosening of parts installed with screws, etc.	· When detected	Retighten with the prescribed tool.

8.2 Preparation for Shipment

When shipping this instrument, if the packing material was saved when the instrument was unpacked, use it to repack the instrument. If the packing material was not saved, pack the instrument as described below. When handling the instrument, always wear clean gloves and handle it gently so that it does not get dented or otherwise damaged.

- (a) Remove dirt and dust from the outside of the instrument with a dry cloth.
- (b) Check that there are no loose or missing screws.
- (c) Protect parts that protrude or may be easily deformed and wrap the instrument in a polyethylene sheet. Also wrap it in waterproofing paper, etc.
- (d) Place the wrapped instrument in a cardboard box and seal the box with adhesive tape. Also consider the shipping distance, shipping means, etc. and place the instrument in a wood crate, as required.

SECTION 8 MAINTENANCE

(Blank)

SECTION 9

TROUBLESHOOTING AND REPAIR

9.1 Before Considering Trouble

If the instrument is not operating properly for some reason, check it as follows:

- **Power is not turned on**

Is the power cord loose? → Plug in firmly.



Is the fuse blown? → Replace the fuse.

- **Synchronization is not established.**

Are the transmit and receive interfaces the same?
(Termination conditions, output level, offset, etc.) → Check the set values and set them to the correct values.



Is the connection cable normal? → Change the cable.



Initialize the instrument. (Transmitter and receiver)
Set the receiver the same as the transmitter.

- **Error added**

Is the cable loose? → Retighten the connector.



Is Error addition OFF? → Set Error addition to OFF.



Are the phase margin and bias margin sufficient? → Adjust so that the phase and offset are suitably cut.

- **Floppy disk drive is not used.**

Is the floppy disk normal ? → Use the normal floppy disk.



Is the head of floppy disk drive dusty ? → Clean head of floppy disk drive with 3.5 inch head cleaning disk set.

If the problem cannot be found from the above check items, contact the service section of Anritsu.

9.2 Fuse Replacement

Turn off the power switch, then disconnect the power cable plugged into the AC power inlet. Next, open the AC power fuse holder cover and replace the fuse with a spare.

SECTION 9 TROUBLESHOOTING AND REPAIR

(Blank)