MX285051A/MX269051A
5G Standard
Measurement Software
(Base License)
Operation Manual

Fifth Edition

- **For safety and warning information, please read this manual before attempting to use the equipment.**
- **Additional safety and warning information is provided within the MS2850A Signal Analyzer Operation Manual (Mainframe Operation) or MS2690A/MS2691A/MS2692A Signal Analyzer Operation Manual (Mainframe Operation). Please also refer to it before using the equipment.**
- **Keep this manual with the equipment.**

ANRITSU CORPORATION

Document No.: M-W3922AE-5.0

Safety Symbols

To prevent the risk of personal injury or loss related to equipment malfunction, Anritsu Corporation uses the following safety symbols to indicate safety-related information. Ensure that you clearly understand the meanings of the symbols BEFORE using the equipment. Some or all of the following symbols may be used on all Anritsu equipment. In addition, there may be other labels attached to products that are not shown in the diagrams in this manual.

Symbols used in manual

⚠ DANGER This indicates a very dangerous procedure that could result in serious injury or death if not performed properly.

⚠ WARNING This indicates a hazardous procedure that could result in serious injury or death if not performed properly.

⚠ CAUTION This indicates a hazardous procedure or danger that could result in light-to-severe injury, or loss related to equipment malfunction, if proper precautions are not taken.

Safety Symbols Used on Equipment and in Manual

The following safety symbols are used inside or on the equipment near operation locations to provide information about safety items and operation precautions. Ensure that you clearly understand the meanings of the symbols and take the necessary precautions BEFORE using the equipment.

This indicates a prohibited operation. The prohibited operation is indicated symbolically in or near the barred circle.

This indicates an obligatory safety precaution. The obligatory operation is indicated symbolically in or near the circle.

This indicates a warning or caution. The contents are indicated symbolically in or near the triangle.

This indicates a note. The contents are described in the box.

These indicate that the marked part should be recycled.

MX285051A/MX269051A
5G Standard Measurement Software (Base License)
Operation Manual

28 April 2017 (First Edition)
30 September 2020 (Fifth Edition)

Copyright © 2017-2020, ANRITSU CORPORATION.
All rights reserved. No part of this manual may be reproduced without the prior written permission of the publisher.
The operational instructions of this manual may be changed without prior notice.
Printed in Japan

Equipment Certificate

Anritsu Corporation guarantees that this equipment was inspected at shipment and meets the published specifications.

Anritsu Warranty

- During the warranty period, Anritsu Corporation will repair or exchange this software free-of-charge if it proves defective when used as described in the operation manual.
- The warranty period is 6 months from the purchase date.
- The warranty period after repair or exchange will remain 6 months from the original purchase date, or 30 days from the date of repair or exchange, depending on whichever is longer.
- This warranty does not cover damage to this software caused by Acts of God, natural disasters, and misuse or mishandling by the customer.

In addition, this warranty is valid only for the original equipment purchaser. It is not transferable if the equipment is resold.

Anritsu Corporation shall assume no liability for damage or financial loss of the customer due to the use of or a failure to use this equipment, unless the damage or loss is caused due to Anritsu Corporation’s intentional or gross negligence.

Anritsu Corporation Contact

In the event of this equipment malfunctions, please contact an Anritsu Service and Sales office. Contact information can be found on the last page of the printed version of this manual, and is available in a separate file on the PDF version.

Notes On Export Management

This product and its manuals may require an Export License/Approval by the Government of the product's country of origin for re-export from your country.
Before re-exporting the product or manuals, please contact us to confirm whether they are export-controlled items or not.
When you dispose of export-controlled items, the products/manuals need to be broken/shredded so as not to be unlawfully used for military purpose.

Software End-User License Agreement (EULA)

Please carefully read and accept this Software End-User License Agreement (hereafter this EULA) before using (includes executing, copying, installing, registering, etc.) this Software (includes programs, databases, scenarios, etc., used to operate, set, etc., Anritsu electronic equipment, etc.). By using this Software, you shall be deemed to have agreed to be bound by the terms of this EULA, and Anritsu Corporation (hereafter Anritsu) hereby grants you the right to use this Software with the Anritsu specified equipment (hereafter Equipment) for the purposes set out in this EULA.

Article 1. Grant of License and Limitations

1. You may not to sell, transfer, rent, lease, lend, disclose, sublicense, or otherwise distribute this Software to third parties, whether or not paid therefor.
2. You may make one copy of this Software for backup purposes only.
3. You are not permitted to reverse engineer, disassemble, decompile, modify or create derivative works of this Software.
4. This EULA allows you to install one copy of this Software on one piece of Equipment.

Article 2. Disclaimers

To the extent not prohibited by law, in no event shall Anritsu be liable for direct, or any incidental, special, indirect or consequential damages whatsoever, including, without limitation, damages for loss of profits, loss of data, business interruption or any other commercial damages or losses, and damages claimed by third parties, arising out of or related to your use or inability to use this Software, unless the damages are caused due to Anritsu's intentional or gross negligence.

Article 3. Limitation of Liability

1. If a fault (bug) is discovered in this Software, failing this Software to operate as described in the operation manual or specifications even though you have used this Software as described in the manual, Anritsu shall at its own discretion, fix the bug, or replace the software, or suggest a workaround, free-of-charge, provided, however, that the faults caused by the following items and any of your lost or damaged data whatsoever shall be excluded from repair and the warranty.
   i) If this Software is deemed to be used for purposes not described in the operation manual or specifications.
   ii) If this Software has been used in conjunction with other non-Anritsu-approved software.
   iii) If this Software or the Equipment has been modified, repaired, or otherwise altered without Anritsu's prior approval.
   iv) For any other reasons out of Anritsu's direct control and responsibility, such as but not limited to, natural disasters, software virus infections, or any devices other than this Equipment, etc.
2. Expenses incurred for transport, hotel, daily allowance, etc., for on-site repairs or replacement by Anritsu engineers necessitated by the above faults shall be borne by you.
3. The warranty period for faults listed in Section 1 of this Article shall be either 6 months from the date of purchase of this Software or 30 days after the date of repair or replacement, whichever is longer.

Article 4. Export Restrictions

You shall not use or otherwise export or re-export directly or indirectly this Software except as authorized by the laws and regulations of Japan and the United States, etc. In particular, this Software shall not be exported or re-exported (a) into any Japan or US embargoed countries or (b) to anyone restricted by the Japanese export control regulations, or the US Treasury Department's list of Specially Designated Nationals or the US Department of Commerce Denied Persons List or Entity List. In using this Software, you warrant that you are not located in any such embargoed countries or on any such lists. You also agree that you will not use or otherwise export or re-export this Software for any purposes prohibited by the Japanese and US laws and regulations, including, without limitation, the development, design and manufacture or production of missiles or nuclear, chemical or biological weapons of mass destruction, and conventional weapons.

Article 5. Change of Terms

Anritsu may change without your approval the terms of this EULA if the changes are for the benefit of general customers, or are reasonable in light of the purpose of this EULA and circumstances of the changes. At the time of change, Anritsu will inform you of those changes and its effective date, as a general rule 45 days, in advance on its website, or in writing or by e-mail.

Article 6. Termination

1. Anritsu may terminate this EULA immediately if you violate any conditions described herein. This EULA shall also be terminated immediately by Anritsu if there is any good reason that it is deemed difficult to continue this EULA, such as your violation of Anritsu copyrights, patents, etc. or any laws and ordinances, or if it turns out that you belong to an antisocial organization or has a socially inappropriate relationship with members of such organization.
2. You and Anritsu may terminate this EULA by a written notice to the other party 30 days in advance.

Article 7. Damages

If Anritsu suffers any damages or loss, financial or otherwise, due to your violation of the terms of this EULA, Anritsu shall have the right to seek proportional damages from you.

Article 8. Responsibility after Termination

Upon termination of this EULA in accordance with Article 6, you shall cease all uses of this Software immediately and shall as directed by Anritsu either destroy or return this Software and any backup copies, full or partial, to Anritsu.

Article 9. Negotiation for Dispute Resolution

If matters of interpretational dispute or items not covered under this EULA arise, they shall be resolved by negotiations in good faith between you and Anritsu.

Article 10. Governing Law and Court of Jurisdiction

This EULA shall be governed by and interpreted in accordance with the laws of Japan without regard to the principles of the conflict of laws thereof, and any disputes arising from or in relation to this EULA that cannot be resolved by negotiation described in Article 9 shall be subject to and be settled by the exclusive agreed jurisdiction of the Tokyo District Court of Japan.

Revision History:

February 29th, 2020

Cautions Against Computer Virus Infection

- Copying files and data
  Only files that have been provided directly from Anritsu or generated using Anritsu equipment should be copied to the instrument.
  All other required files should be transferred by means of USB flash drive or CompactFlash media after undergoing a thorough virus check.
- Adding software
  Do not download or install software that has not been specifically recommended or licensed by Anritsu.
- Network connections
  Ensure that the network has sufficient anti-virus security protection in place.
- Protection against malware (malicious software such as viruses).
  This equipment runs on Windows Operating System.
  To connect this equipment to network, the following is advised.
  - Activate Firewall.
  - Install important updates of Windows.
  - Use antivirus software.

About This Manual

■ **Composition of Operation Manuals**

The operation manuals for the MX285051A/MX269051A 5G Standard Measurement Software are comprised as shown in the figure below.

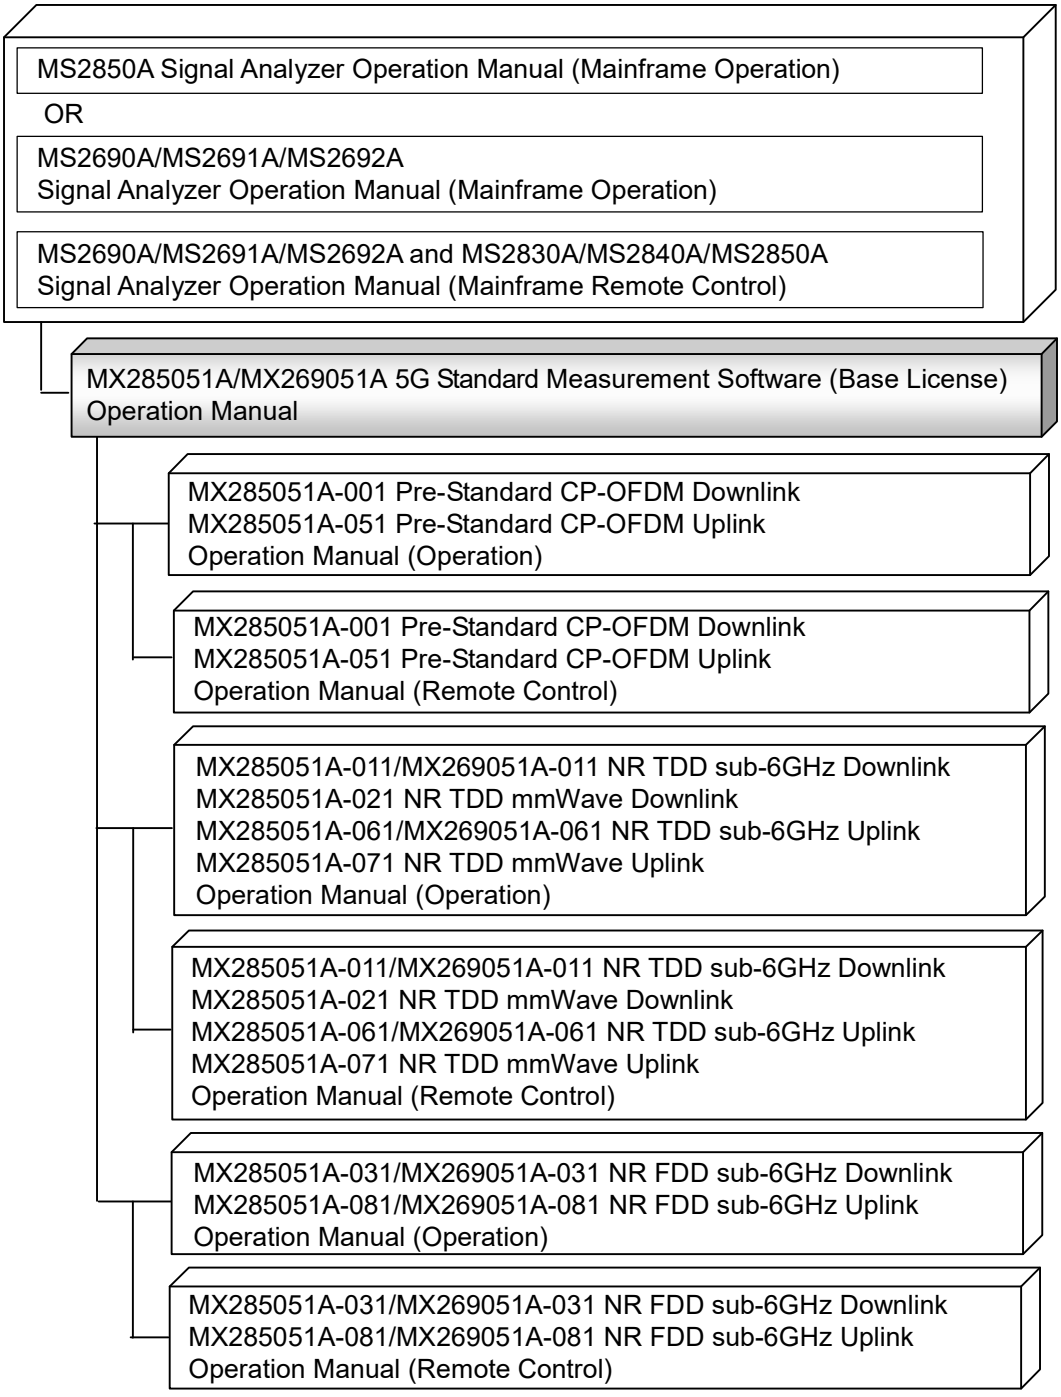

- Signal Analyzer Operation Manual (Mainframe Operation)
- Signal Analyzer Operation Manual (Mainframe Remote Control)

These manuals describe basic operating methods, maintenance procedures, common functions, and common remote control of the signal analyzer mainframe.

- 5G Standard　Measurement Software (Base License) Operation Manual <This document>

This manual describes basic operating methods, and functions of the 5G Standard　Measurement Software (Base License).

- MX285051A-001 Pre-Standard CP-OFDM Downlink
  MX285051A-051 Pre-Standard CP-OFDM Uplink
  Operation Manual (Operation)

This manual describes basic operating methods, and functions.

- MX285051A-001 Pre-Standard CP-OFDM Downlink
  MX285051A-051 Pre-Standard CP-OFDM Uplink
  Operation Manual (Remote Control)

This manual describes remote control.

- MX285051A-011/MX269051A-011 NR TDD sub-6GHz Downlink
  MX285051A-021 NR TDD mmWave Downlink
  MX285051A-061/MX269051A-061 NR TDD sub-6GHz Uplink
  MX285051A-071 NR TDD mmWave Uplink
  Operation Manual (Operation)

This manual describes basic operating methods, and functions.

- MX285051A-011/MX269051A-011 NR TDD sub-6GHz Downlink
  MX285051A-021 NR TDD mmWave Downlink
  MX285051A-061/MX269051A-061 NR TDD sub-6GHz Uplink
  MX285051A-071 NR TDD mmWave Uplink
  Operation Manual (Remote Control)

This manual describes remote control.

- MX285051A-031/MX269051A-031 NR FDD sub-6GHz Downlink
  MX285051A-081/MX269051A-081 NR FDD sub-6GHz Uplink
  Operation Manual (Operation)

This manual describes basic operating methods, and functions.

- MX285051A-031/MX269051A-031 NR FDD sub-6GHz Downlink
  MX285051A-081/MX269051A-081 NR FDD sub-6GHz Uplink
  Operation Manual (Remote Control)

This manual describes remote control.

As for signal analyzer hardware and its basic functions and operation outline, refer to *MS2850A Signal Analyzer Operation Manual (Mainframe Operation) or MS2690A/MS2691A/MS2692A Signal Analyzer Operation Manual (Mainframe Operation)*.

As for signal analyzer application's basic remote control functions and its definitions of common commands, refer to *MS2690A/MS2691A/MS2692A and MS2830A/MS2840A/MS2850A Signal Analyzer Operation Manual (Mainframe Remote Control)*.

Convention Used in This Manual

In this document, indicates a panel key.

Throughout this document, the use of MS2850A is assumed unless otherwise specified. If using MS2690A/MS2691A/MS2692A (hereinafter, MS269xA), change MS2850A to read MS269xA.

Table of Contents

About This Manual..... I

Chapter 1 Overview..... 1-1

1.1 Product Overview 1-2
1.2 Product Configuration 1-3

Chapter 2 Preparation..... 2-1

2.1 Signal Path Setup 2-2
2.2 Application Startup and Selection..... 2-4
2.3 Initialization and Calibration..... 2-5

Chapter 3 Measurement 3-1

3.1 Basic Operation 3-2

Chapter 1 Overview

This chapter provides an overview of the MX285051A/MX269051A 5G Standard Measurement Software (Base License) and describes the product configuration.

1.1 Product Overview 1-2
1.2 Product Configuration 1-3
1.2.1 Standard configuration 1-3
1.2.2 Option 1-3
1.2.3 Applicable parts 1-4

1.1 Product Overview

The MS2850A or MS269xA Signal Analyzer enables high-speed, high-accuracy, and simple measurements of transmission characteristics of base stations and mobile stations for various mobile communications types. The MS2850A or MS269xA is equipped with high-performance signal analyzer and spectrum analyzer functions as standard, with optional measurement software allowing modulation analysis functionality supporting various digital modulation modes.

The MX285051A/MX269051A 5G Standard Measurement Software (Base License) (hereinafter, referred to as "MX285051A/MX269051A") allows measuring RF characteristics according to 5G standard by installing the software options such as MX285051A-001 Pre-Standard CP-OFDM Downlink.

Note:

One of the following software options is required to use the MX285051A/MX269051A.

- MX285051A-001 Pre-Standard CP-OFDM Downlink
- MX285051A-051 Pre-Standard CP-OFDM Uplink
- MX285051A-011/MX269051A-011 NR TDD sub-6GHz Downlink
- MX285051A-061/MX269051A-061 NR TDD sub-6GHz Uplink
- MX285051A-021 NR TDD mmWave Downlink
- MX285051A-071 NR TDD mmWave Uplink
- MX285051A-031/MX269051A-031 NR FDD sub-6GHz Downlink
- MX285051A-081/MX269051A-081 NR FDD sub-6GHz Uplink

1.2 Product Configuration

1.2.1 Standard configuration

Table 1.2.1-1 or Table 1.2.1-2 lists the standard configuration of the MX285051A/MX269051A.

Table 1.2.1-1 Standard configuration (MS2850A)

Item	Model Name	Product Name	Q'ty	Remarks
Application	MX285051A	5G Standard Measurement Software (Base License)	1	
Accessory	—	Installation CD-ROM	1	Application software, operation manual CD-ROM

Table 1.2.1-2 Standard configuration (MS269xA)

Item	Model Name	Product Name	Q'ty	Remarks
Application	MX269051A	5G Standard Measurement Software (Base License)	1	
Accessory	—	Installation CD-ROM	1	Application software, operation manual CD-ROM

1.2.2 Option

Tables 1.2.2-1 or Tables 1.2.2-2 lists the option for the MX285051A/MX269051A. This is sold separately.

Table 1.2.2-1 Option (MS2850A)

Option No.	Product Name	Remarks
MX285051A-001	Pre-Standard CP-OFDM Downlink	
MX285051A-051	Pre-Standard CP-OFDM Uplink	
MX285051A-011	NR TDD sub-6GHz Downlink	
MX285051A-061	NR TDD sub-6GHz Uplink	
MX285051A-021	NR TDD mmWave Downlink	
MX285051A-071	NR TDD mmWave Uplink	
MX285051A-031	NR FDD sub-6GHz Downlink	
MX285051A-081	NR FDD sub-6GHz Uplink	

Table 1.2.2-2 Option (MS269xA)

Option No.	Product Name	Remarks
MX269051A-011	NR TDD sub-6GHz Downlink	
MX269051A-061	NR TDD sub-6GHz Uplink	
MX269051A-031	NR FDD sub-6GHz Downlink	
MX269051A-081	NR FDD sub-6GHz Uplink	

1.2.3 Applicable parts

Table 1.2.3-1 lists the applicable parts for the MX285051A/MX269051A.

Table 1.2.3-1 Applicable parts

Model Name	Product Name	Remarks
W3922AE	MX285051A/MX269051A 5G Standard Measurement Software (Base License) Operation Manual	English, printed version

Chapter 2 Preparation

This chapter describes the preparations required for using the MX285051A/MX269051A you are using.
Refer to *MS2850A Signal Analyzer Operation Manual (Mainframe Operation)* or *MS2690A/MS2691A/MS2692A Signal Analyzer Operation Manual (Mainframe Operation)* for common features, the panel keys, connectors used to connect external devices and general points of caution not included in this manual.

2.1 Signal Path Setup 2-2
2.2 Application Startup and Selection 2-4
2.2.1 Launching application 2-4
2.2.2 Selecting application 2-4
2.3 Initialization and Calibration 2-5
2.3.1 Initialization 2-5
2.3.2 Calibration 2-5

2.1 Signal Path Setup

As shown in Figure 2.1-1, connect the mainframe and the DUT using an RF cable, so that the signal to be tested is input to the RF Input connector.

⚠ CAUTION

Do not input a signal that has an excessive level to the RF Input connector.

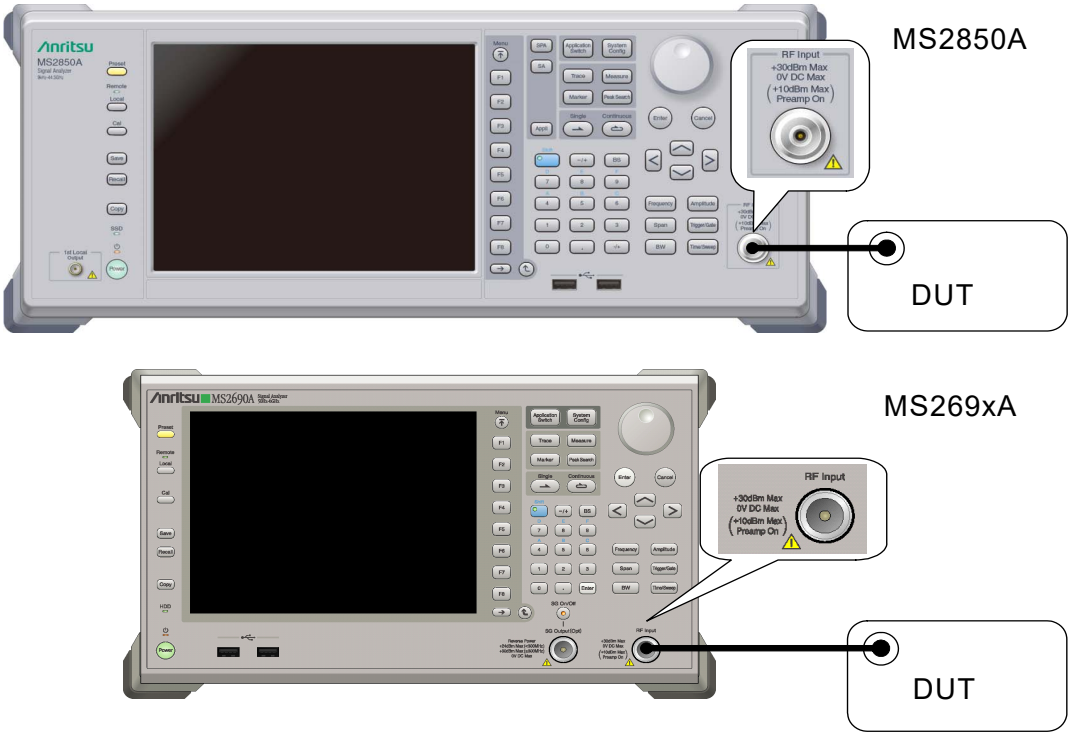

Figure 2.1-1 Signal path setup example

Set the reference signal from external sources, as required.

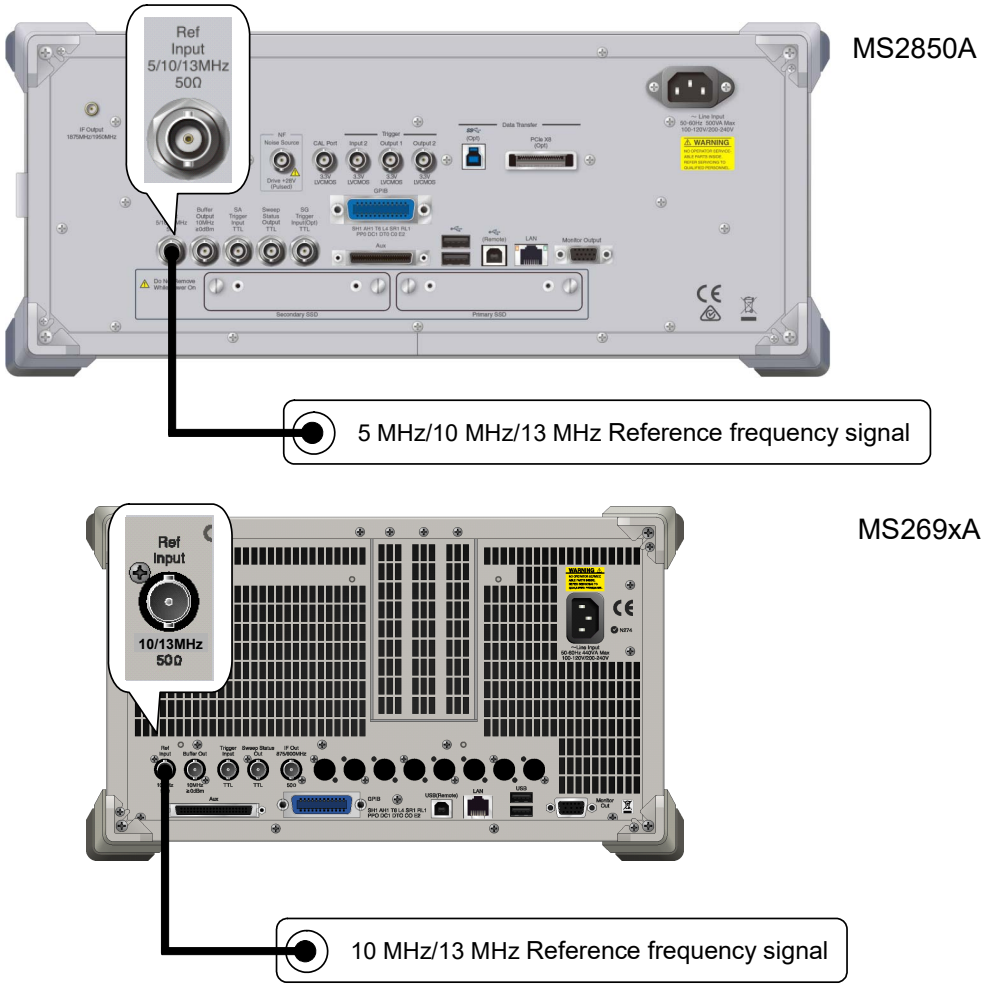

Figure 2.1-2 External reference signal input

2.2 Application Startup and Selection

To use the MX285051A/MX269051A, it is necessary to load (start up) and select the MX285051A/MX269051A.

2.2.1 Launching application

The MX285051A/MX269051A startup procedure is described below.

Note:

The XXX indicates the MX285051A/MX269051A name currently in use.

■ Procedure

1. Press System Config to display the Configuration screen.
2. Press F4 (Application Switch Settings) to display the Application Switch Registration screen.
3. Press F1 (Load Application Select), and move the cursor to "XXX" in the Unloaded Applications list.
   - If "XXX" is displayed in the **Loaded Applications** list, this means that the application is already loaded.
   - If "XXX" appears in neither the **Loaded Applications** nor **Unloaded Applications** list, this means that the application has not been installed.
4. Press F7 (Set) to load the application. If "XXX" is displayed in the **Loaded Applications** list, this means that the application is already loaded.

2.2.2 Selecting application

The selection procedure is described below.

■ Procedure

1. Press Application Switch to display the Application Switch menu.
2. Press the menu function key displaying "XXX".
   - The application can also be selected with mouse, by clicking "XXX" on the task bar.

2.3 Initialization and Calibration

This section describes the parameter settings and the preparations required before starting measurement.

2.3.1 Initialization

After selecting the MX285051A/MX269051A, first perform initialization. Initialization should be performed in order to return the settable parameters to their default settings.

The initialization procedure is as follows.

■ Procedure

1. Press Preset to display the Preset function menu.
2. Press F1 (Preset).

2.3.2 Calibration

Perform calibration before measurement. Calibration sets the level accuracy frequency characteristics for the input level to flat, and adjusts level accuracy deviation caused by internal temperature fluctuations. Calibration should be performed when first performing measurement after turning on power, executes the performance test, or if beginning measurement when there is a difference in ambient temperature from the last time calibration was performed.

■ Procedure

1. Press Cal to display the Application Cal function menu.
2. Press F1 (SIGANA All).

For details on calibration functionality executable, refer to *MS2850A Signal Analyzer Operation Manual (Mainframe Operation)* or *MS2690A/MS2691A/MS2692A Signal Analyzer Operation Manual (Mainframe Operation)*.

Chapter 3 Measurement

This chapter describes the measurement function, the parameter contents and setting methods for the MX285051A/MX269051A.

3.1 Basic Operation 3-2
3.1.1 Screen layout 3-2
3.1.2 Performing measurement 3-3

3.1 Basic Operation

3.1.1 Screen layout

This section describes the screen layout for the MX285051A/MX269051A.

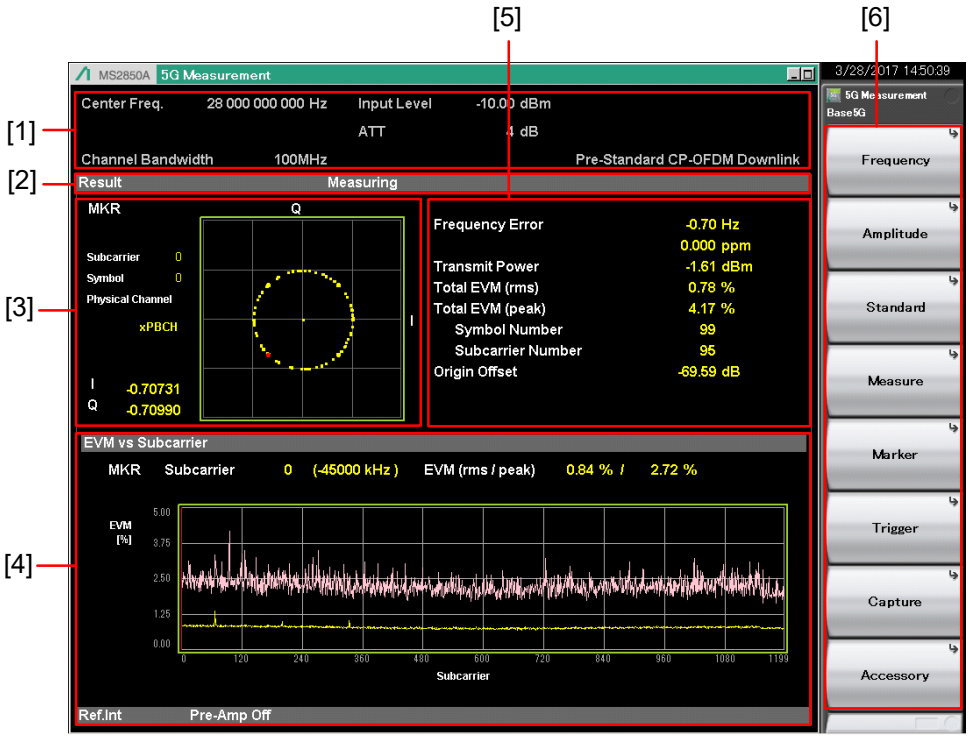

Figure 3.1.1-1 Screen Layout

[1] Measurement parameter

Displays the set parameters.

[2] Status message

Displays the status of signals.

[3] Constellation

Displays a constellation of the selected symbol.

[4] Graph window

Displays a graph of the measurement results.

[5] Result window

Displays measurement results.

[6] Function menu

Displays the functions executable with the function keys.

3.1.2 Performing measurement

Because MX285051A/MX269051A itself does not have measurement functions, a software option must be installed in MX285051A/MX269051A to perform measurement. For details about the measurement functions, see the operation manual for each software option.